



Using Helium Leak Detection CCI Testing to Inform Container Closure System Design

A Prefilled Syringe Case Study

Container Closure Integrity: Regulations, Test Methods, Application
Vienna, Austria; 9-10 November 2017


Allison Dill
Lei Li
Eli Lilly and Company

- ❑ Overview of Helium Leak Detection (HeLD)

- ❑ Method development for syringes
 - Fixture design
 - Helium charging


- ❑ Applications of Helium Leak Detection
 - Determination of inherent package integrity
 - Evaluation of syringe system and sub-system design
 - Assessment of container closure robustness

- **Sensitivity & Quantitative**
 - Mass spectrometer as detector
- **Selectivity**
 - Low atmospheric interference: Helium in the atmosphere (~5 ppm)
 - Do need to minimize lab ambient helium and permeation
- **Flows through cracks ~2.7x faster than air**

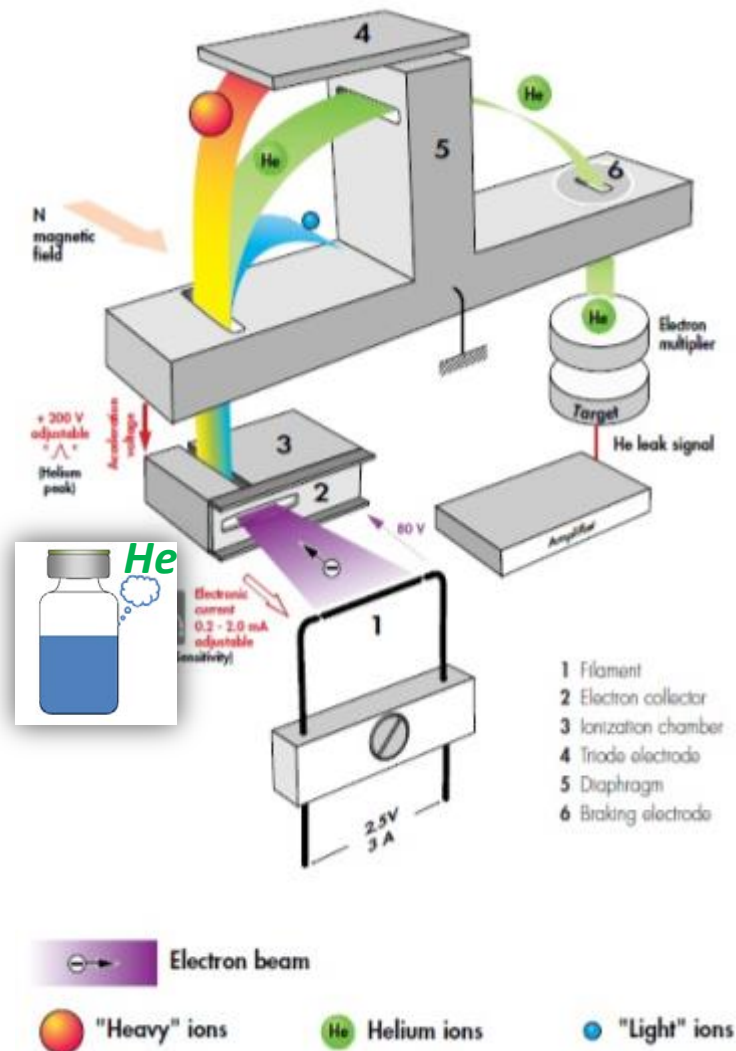


Leak Detection Associates, Blackwood, NJ

- **Calibration**
 - Internal calibration standards
 - Quantitation Range: 1×10^{-11} to 1×10^{-3} atm-cc/sec
- **System suitability**
 - NIST-traceable standard leaks
 - Verified range: 4×10^{-10} to 6×10^{-4} atm-cc/sec
- Results reported as helium leak rate
 - Converted to a nominal leak orifice size using USP <1207> method, where appropriate

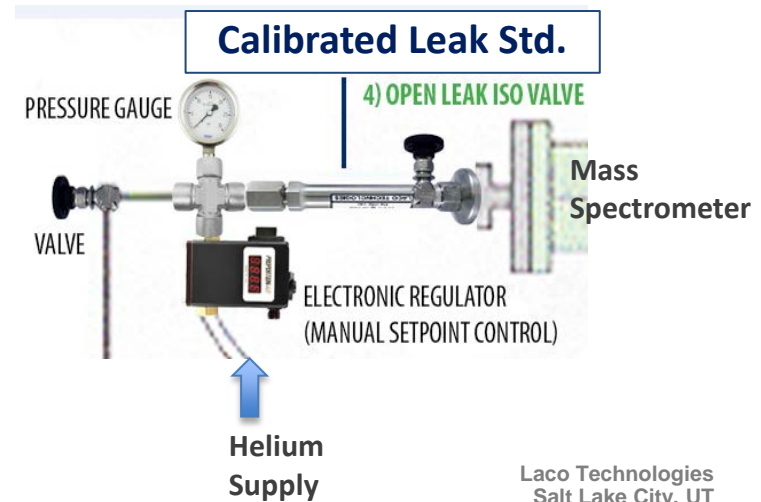

Laco Technologies
Salt Lake City, UT

- **Quantitatively determine inherent package integrity**
 - The leakage rate (or the equivalent leak size) of a well-assembled package using no-defect components. Inherent package integrity is a measure of the leak tightness of a container–closure system, given anticipated variables of material composition, dimension, processing, assembly; package storage, distribution and use.
(*USP<1207>*)
- **Demonstrate conformance to Maximum Allowed Leakage Rate (MALL)**
 - To preserve sterility and product formulation content
 $MALL \leq 6 \times 10^{-6} \text{ mbar} \cdot \text{L/s (atm-cc/sec)}$ (*USP<1207>*)
- **Inform packaging system design and process development**
 - Assess critical seal elements, sub-systems, and system design
 - Evaluate sealing robustness (e.g. impact of potential defects on package integrity)




Drug Product Compartment

- Plunger-barrel seal
- Needle shield seal
 - Needle tip seal
 - Glued needle stem
 - Needle shield/syringe head

Needle Stem Compartment

- Needle shield/syringe head

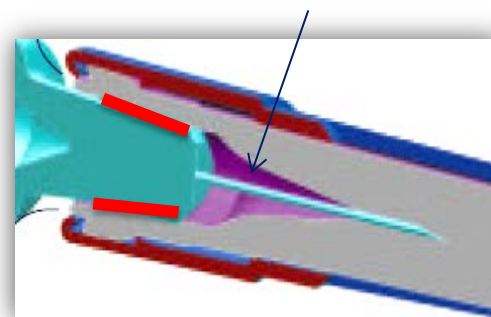


1. **Filling:** syringes charged with helium and plungered in a glove box





2. **Testing:** filled syringe is placed in a sample chamber for testing

- A plunger rod is used to retain plunger during testing

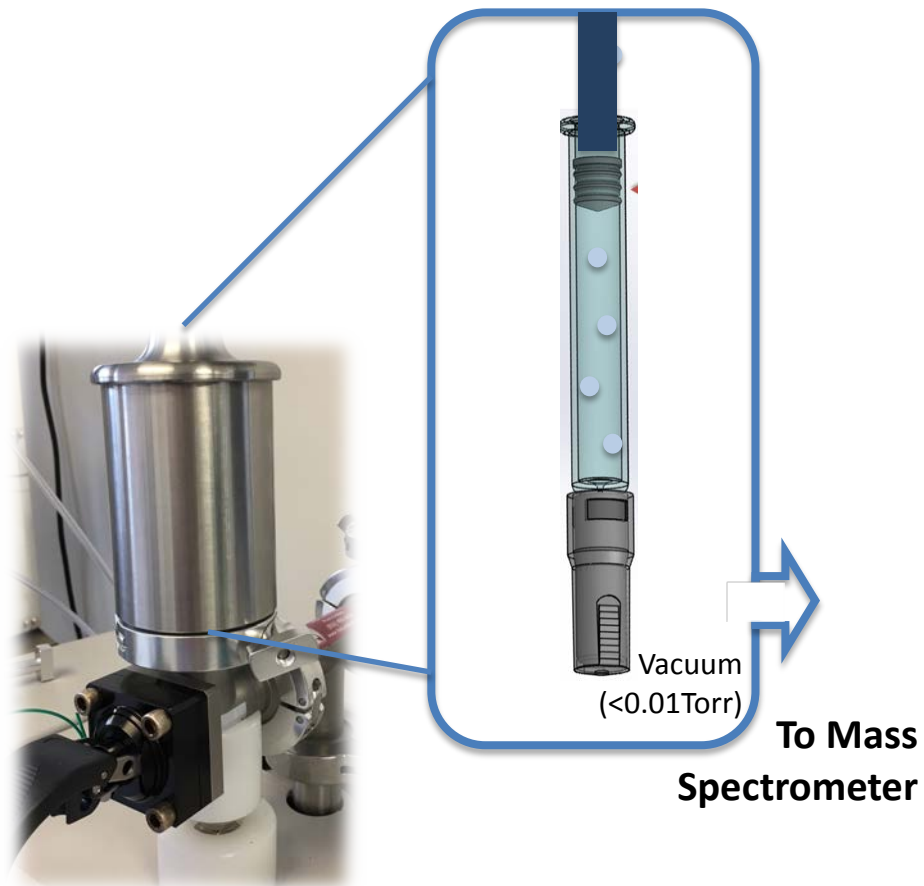


Potential Interferences

- **Desorption** of exterior surface-adsorbed helium
- Helium **permeation**

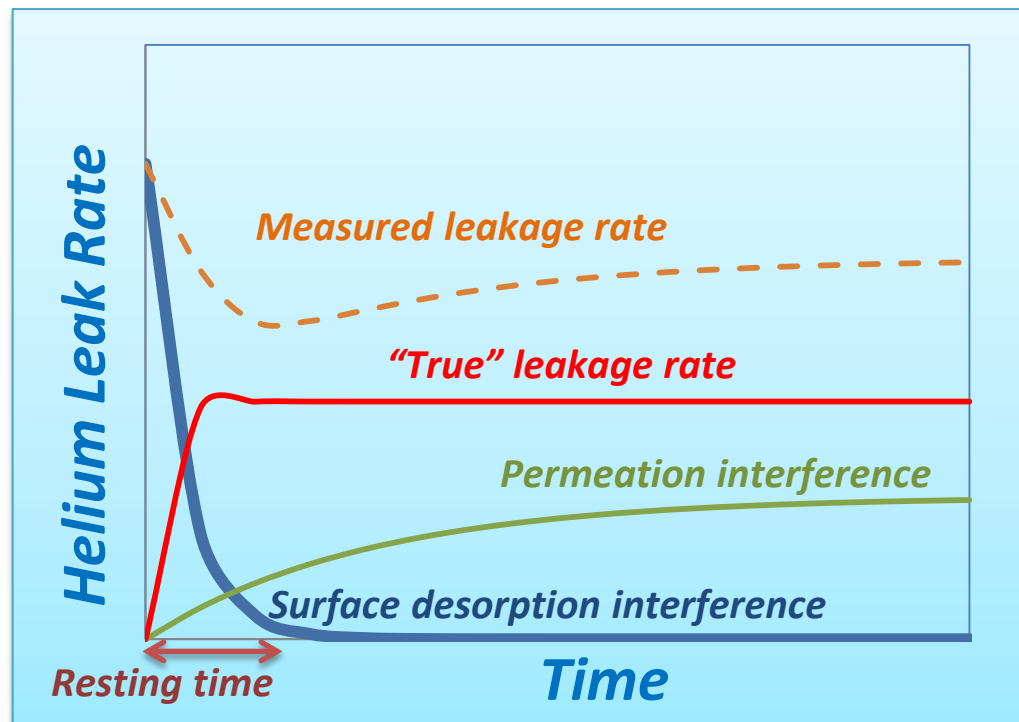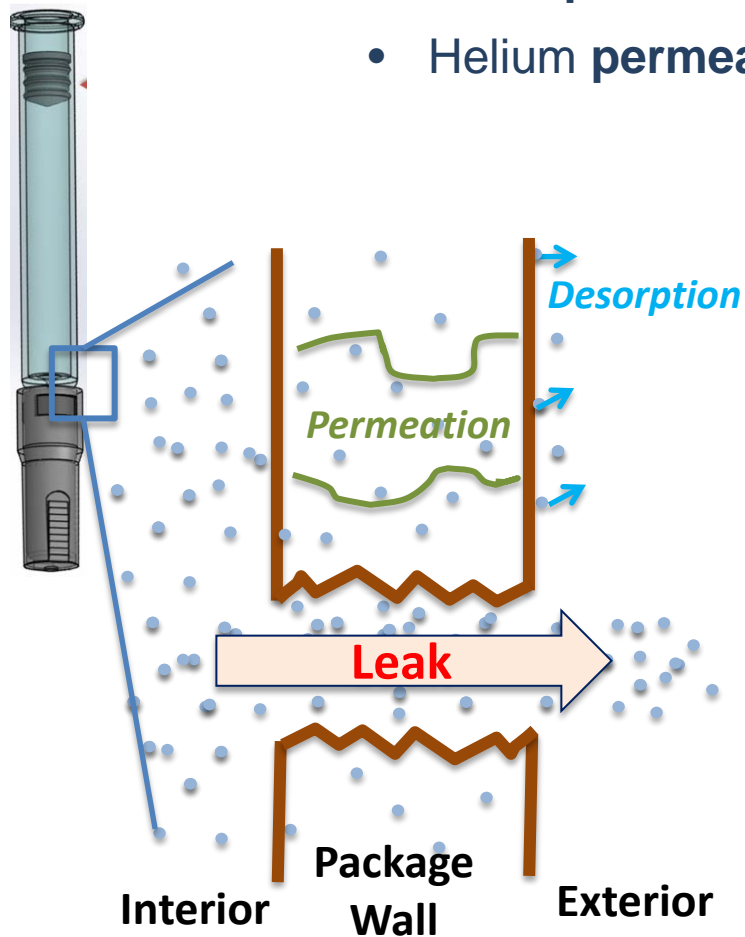

- ✓ **Estimated overall leakage rate**
 - Results can be artificially high due to surface desorption and permeation
- ✓ **Demonstrated conformance to MALL**

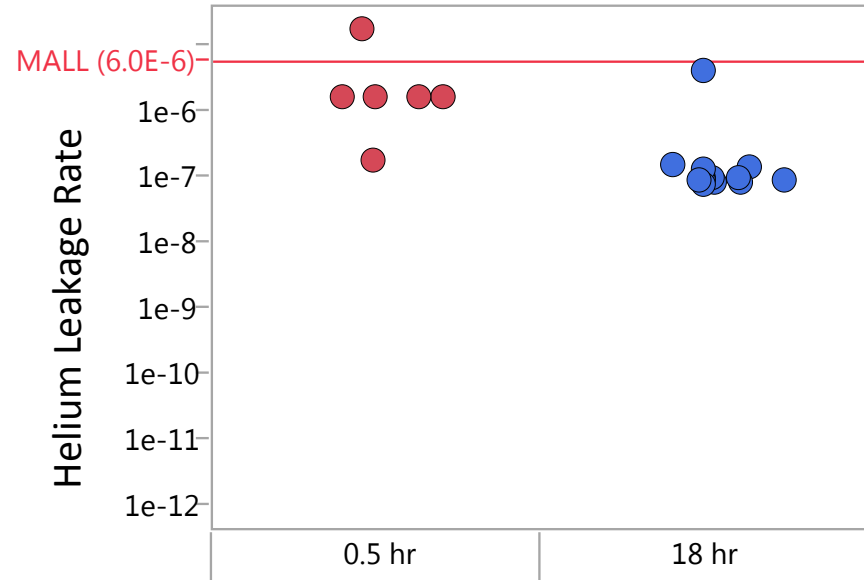

Improvement Needs

- ❑ Reduce helium background noise to measure “true” leakage rate
 - Exterior surface desorption
 - Permeation
- ❑ Need to evaluate sealing capability of critical seal elements and sub-systems

- ❑ **“Fast and Clean”** helium charging
 - **Fast:** allow testing to start prior to significant permeation
 - **Clean:** eliminate helium contact with interfering sample surfaces

- ❑ **“Divide and Conquer”** critical seal elements
 - Isolate critical seal elements for independent assessment






Minimize permeation




Eliminating surface desorption

Key Enabler: Sample Fixture Design

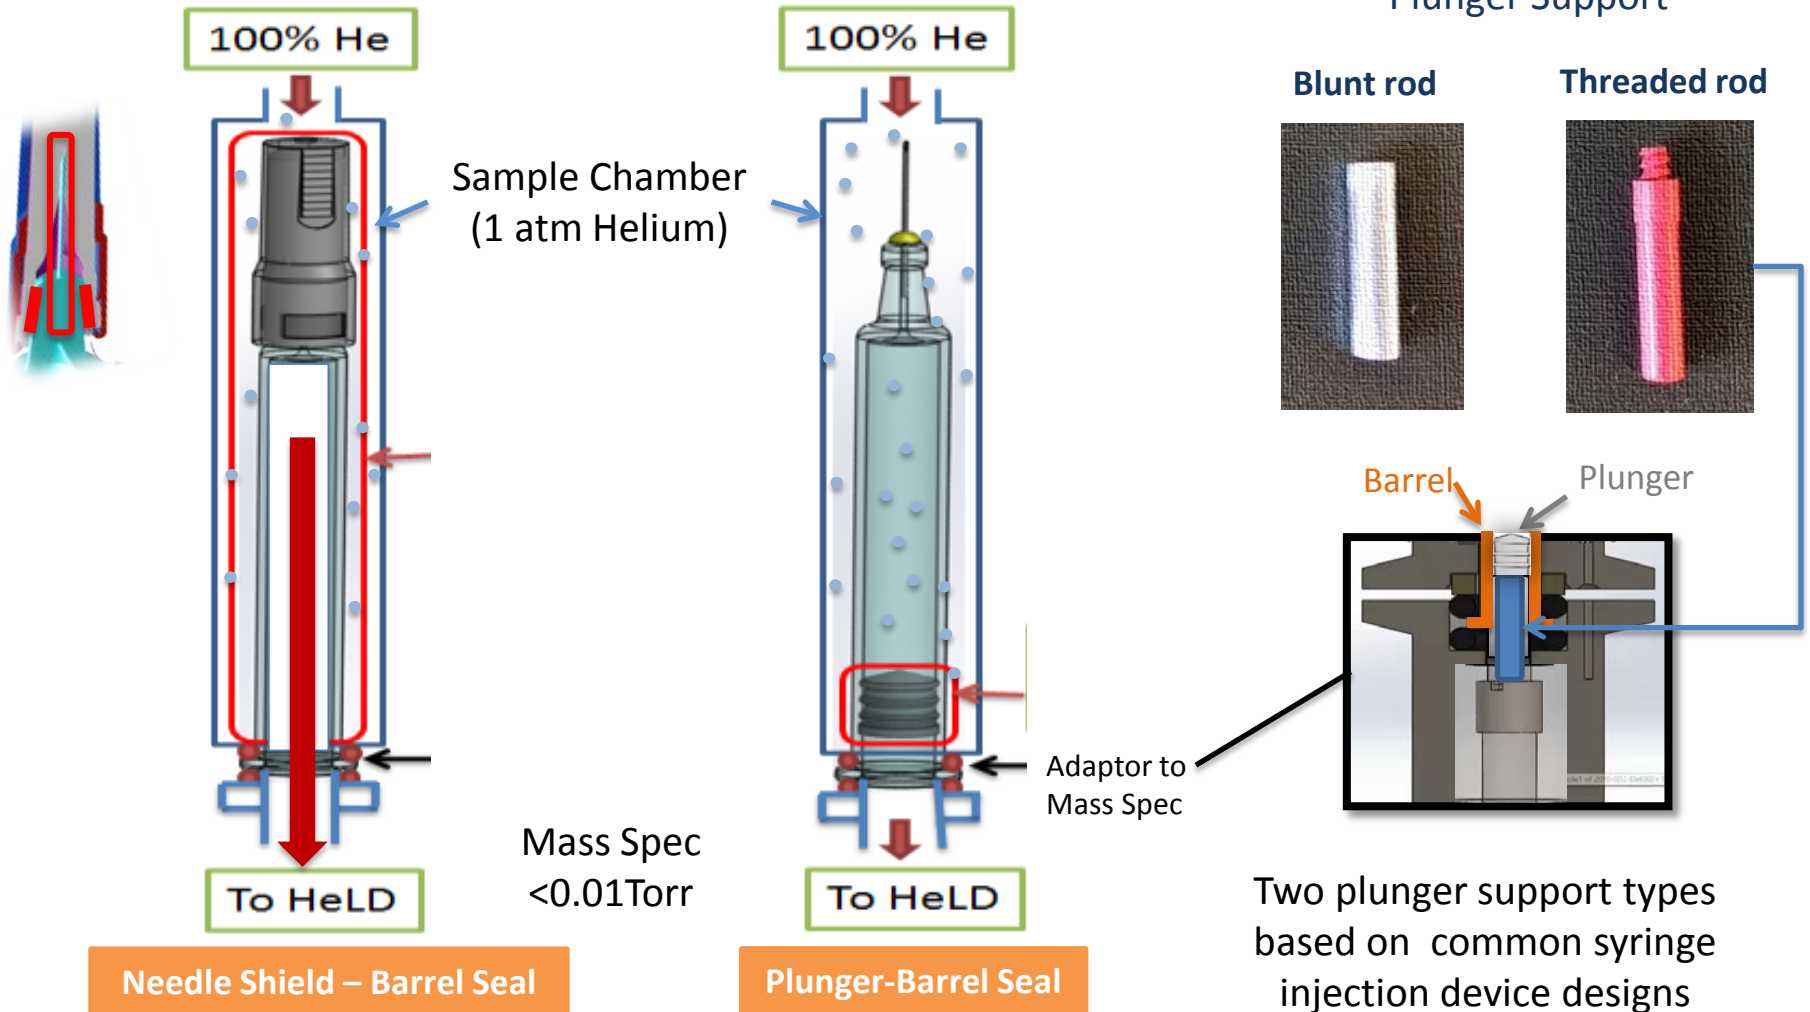

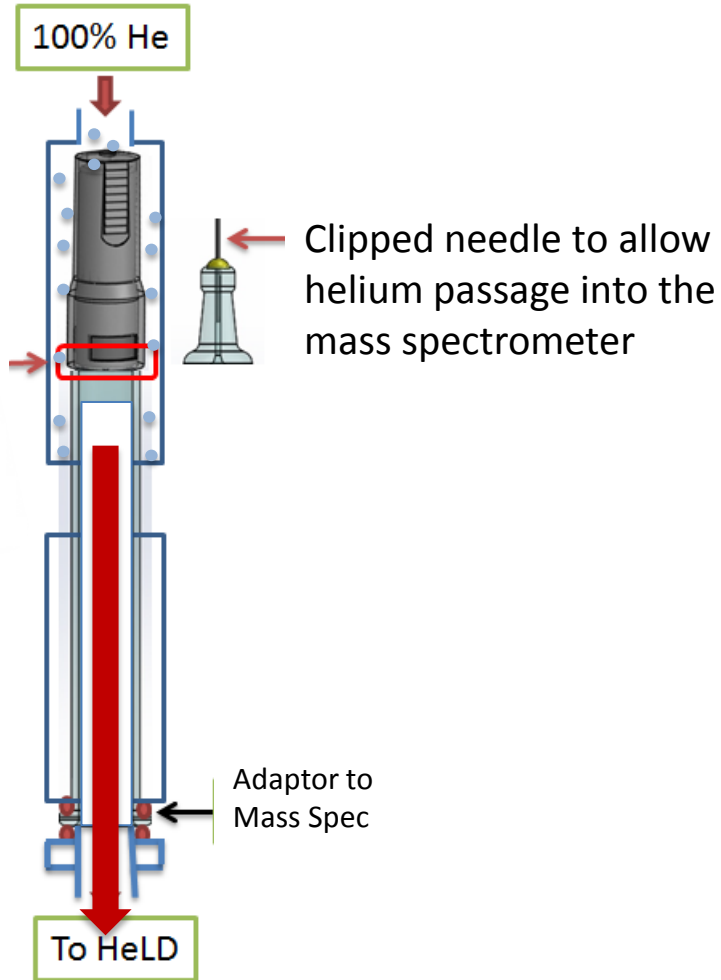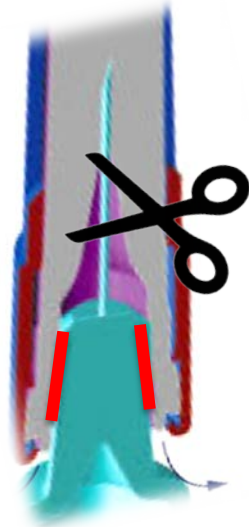


Needle Shield – Barrel head Seal

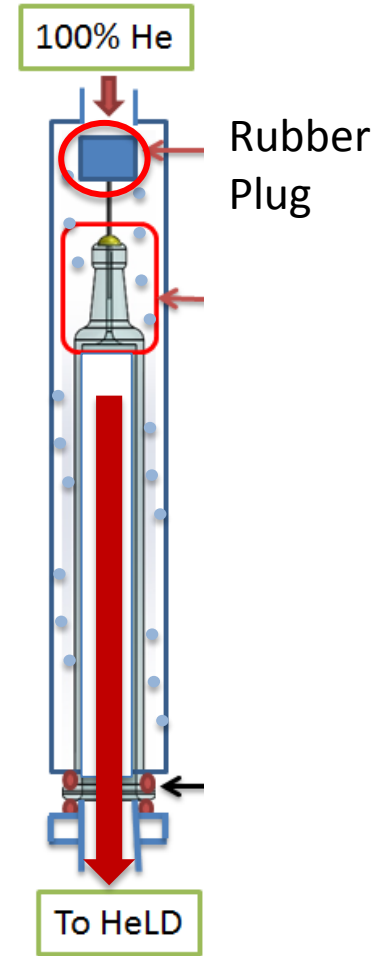

Needle Stem Seals


Fast & Clean Charging of Helium

Goal: to achieve consistent 100% helium charging in the sample chamber to allow accurate quantitative leakage rate testing

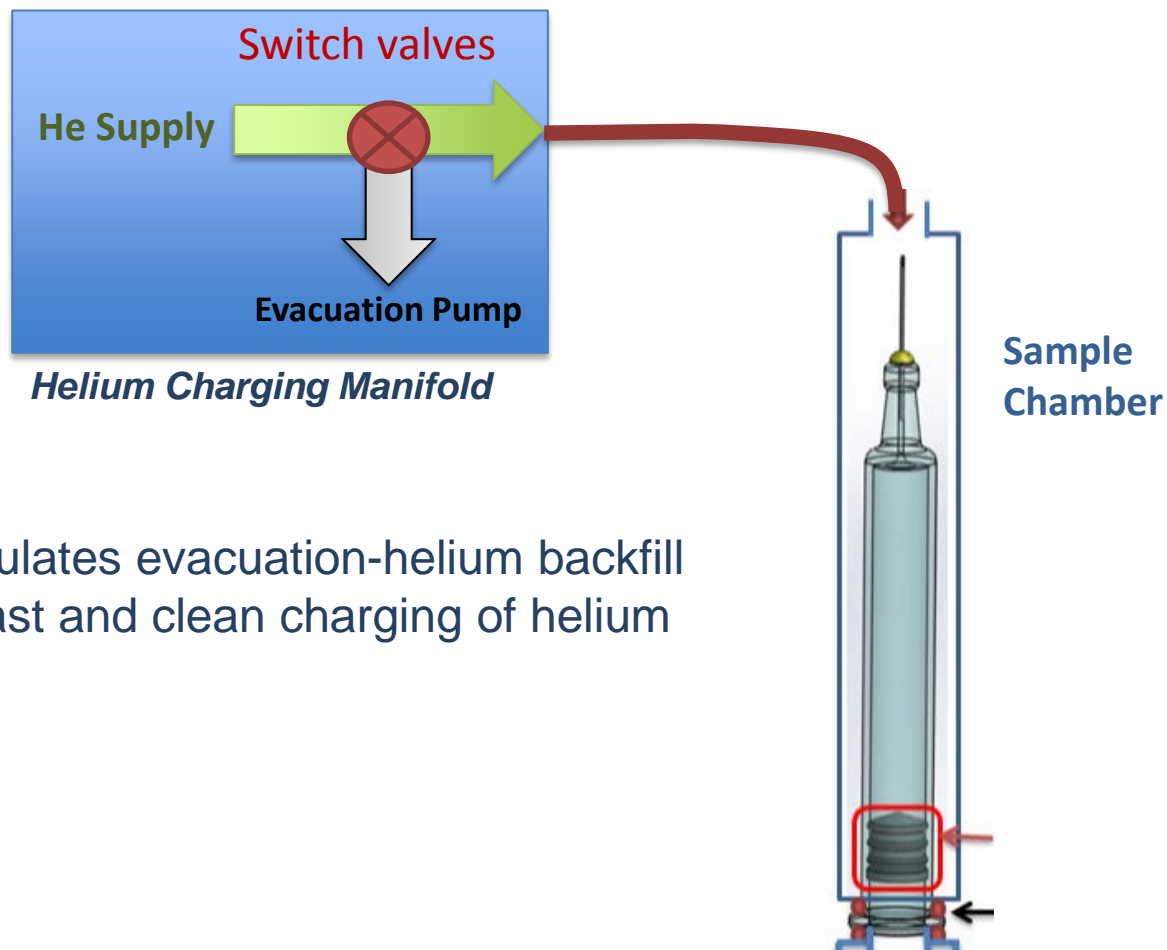

Manifold design regulates evacuation-helium backfill cycles to achieve fast and clean charging of helium


Leakage Rates dependence on He% in Sample Chamber

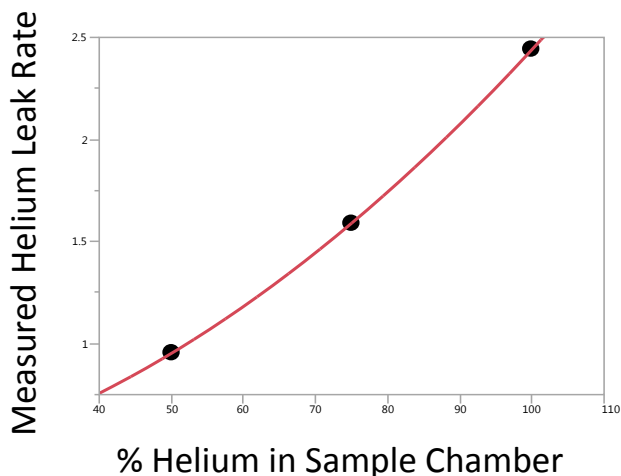

Key Parameters



- Charging cycle
 - Evacuation time (sec)
 - He back-fill time (sec)
- Number of Cycles
- Post-charging testing time (sec)

Leakage Rates vs. Charging Parameters Study


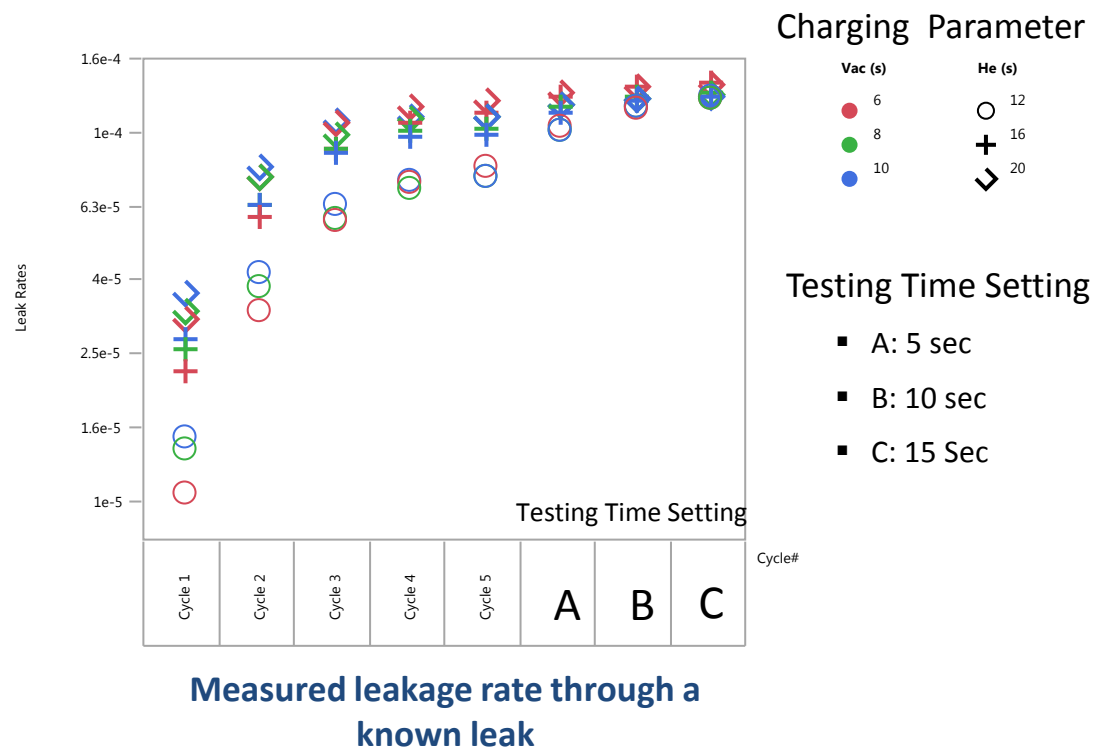


Physically mated (compression) seal

– Critical to product sterility and formulation content protection

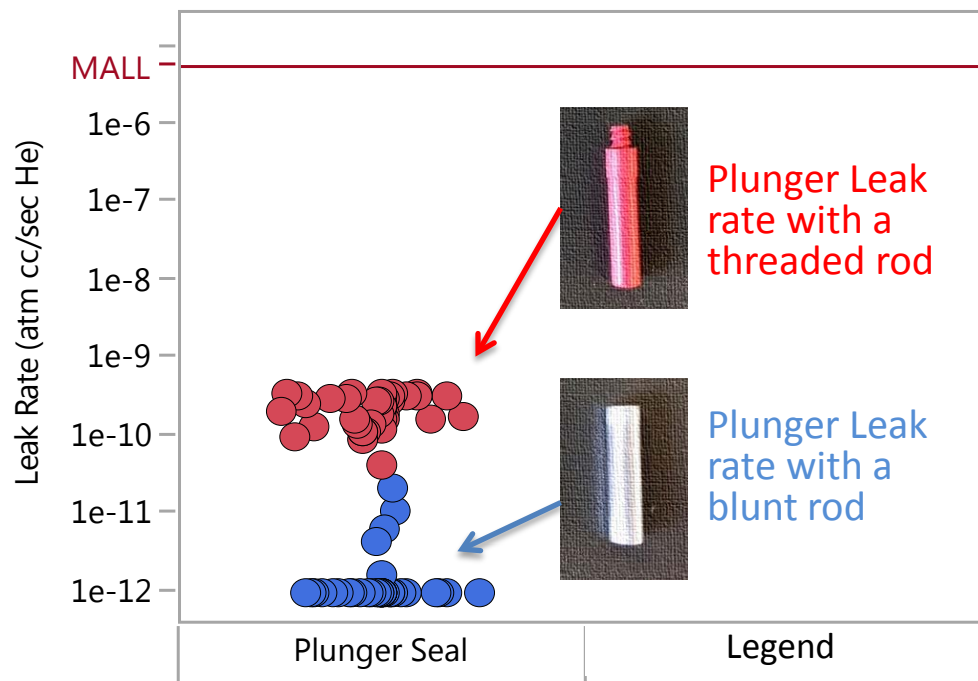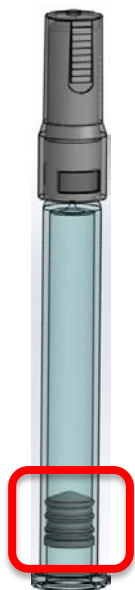

Sample Chamber
(1 atm Helium)

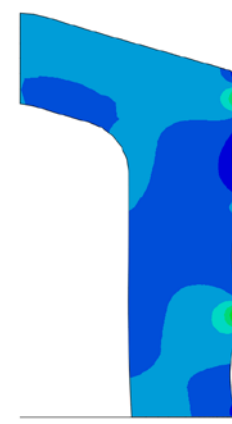


Mass Spec <0.01Torr


- Leakage rate $\leq 4 \times 10^{-10}$ atm-cc/sec
 - Confirm to MALL for preserving sterility and product formulation content
- Plunger rod selection affects plunger seal during testing
 - In agreement with FEA modeling results

A combination of 3 seal elements

- Needle shield – Syringe head
 - Needle tip – Needle shield
 - Glued staked needle
- Critical to product sterility and formulation content protection

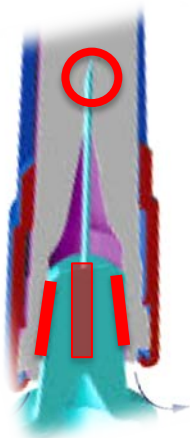


Leak Rate (atm cc/sec He)

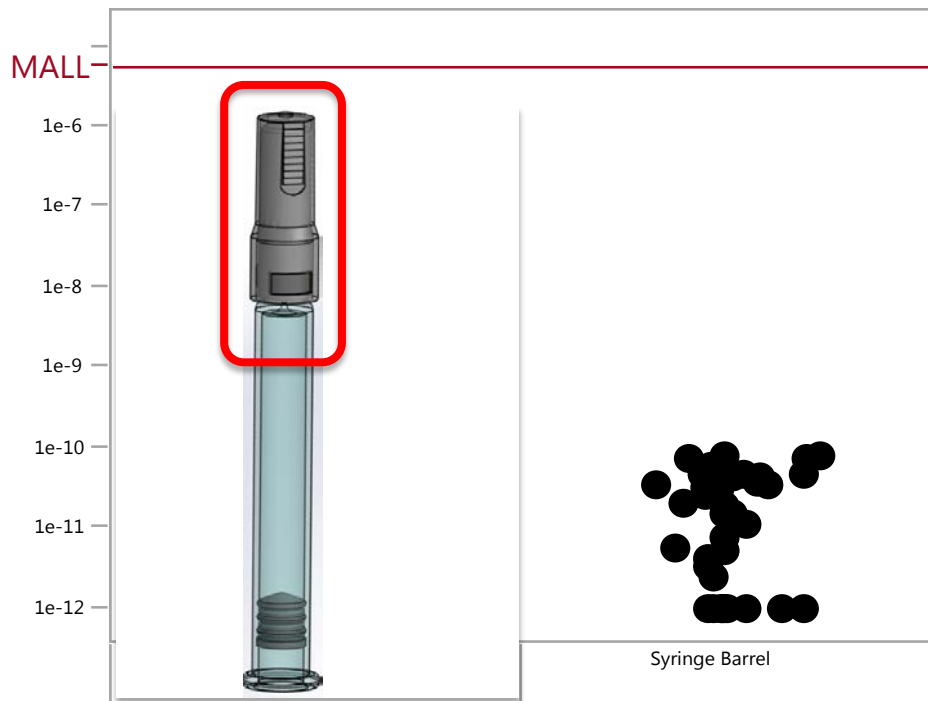


Leakage Rate $\leq 8 \times 10^{-11}$ atm-cc/sec

- Confirm to MALL for preserving sterility and product formulation content

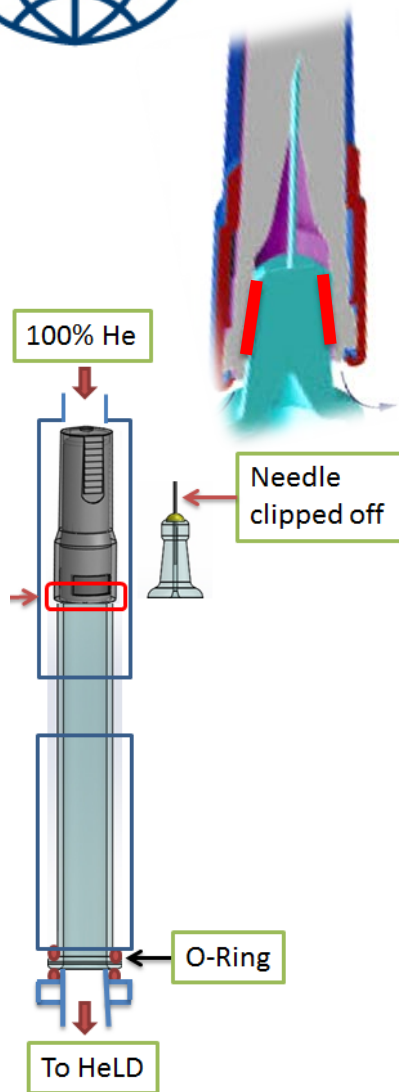

- **Physically mated (compression) seal**
 - Critical to needle stem sterility protection
 - Contributes to DP compartment seal


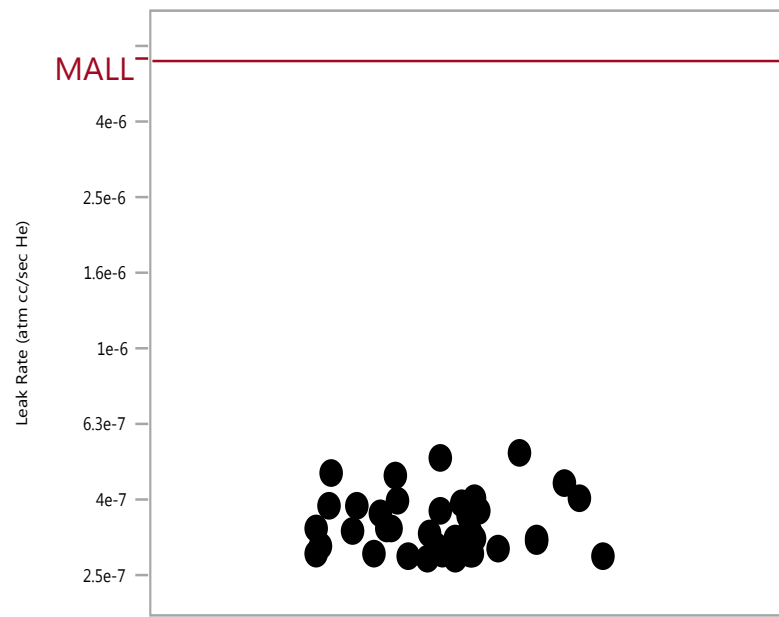


Leakage Rate $\leq 6 \times 10^{-7}$ atm-cc/sec

- Confirm to MALL for preserving sterility

Evaluation of Needle Stem Seals

- Glued (physicochemically bonded) at the base
- Physically mated (compression) seal at the tip
 - Not definitive sterility barriers
 - Poor seals may result to product loss or injection issues

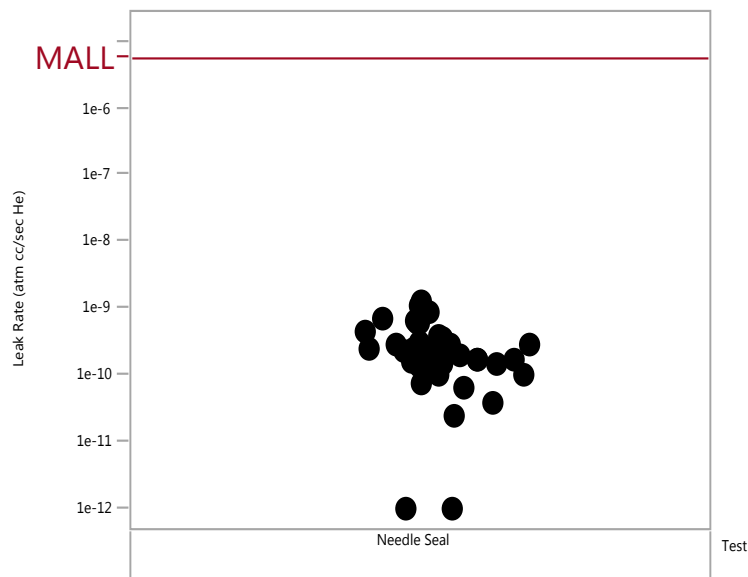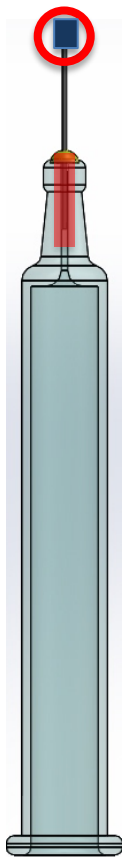



Leakage Rate $\leq 2 \times 10^{-9}$ atm-cc/sec

- Confirm to MALL for preserving sterility and product formulation content

Inherent Package Integrity Summary

- DP compartment (Plunger & Needle Shield) $\leq 5 \times 10^{-10}$ atm-cc/sec
- Needle stem compartment $\leq 6 \times 10^{-7}$ atm-cc/sec
- All individual critical seals conform to MALL

8×10^{-11} atm-cc/sec

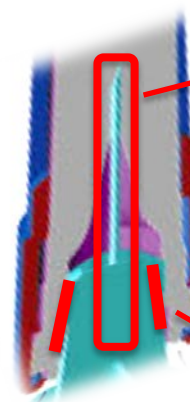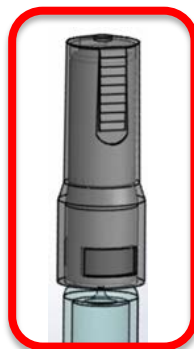


2×10^{-9} atm-cc/sec

6×10^{-7} atm-cc/sec

“Layered” seal design in needle shield significantly lowers overall leakage rate

– Added protection to drug product


4×10^{-10} atm-cc/sec



The needle shield – barrel head seal is the weakest among all seals

Package Integrity was verified for preserving sterility and formulation content


- Each plunger rib assessed individually for sealing capability
 - Assessed by compromising 2 of the 3 ribs, leaving 1 intact rib
 - Evaluate impact of potential plunger molding defects

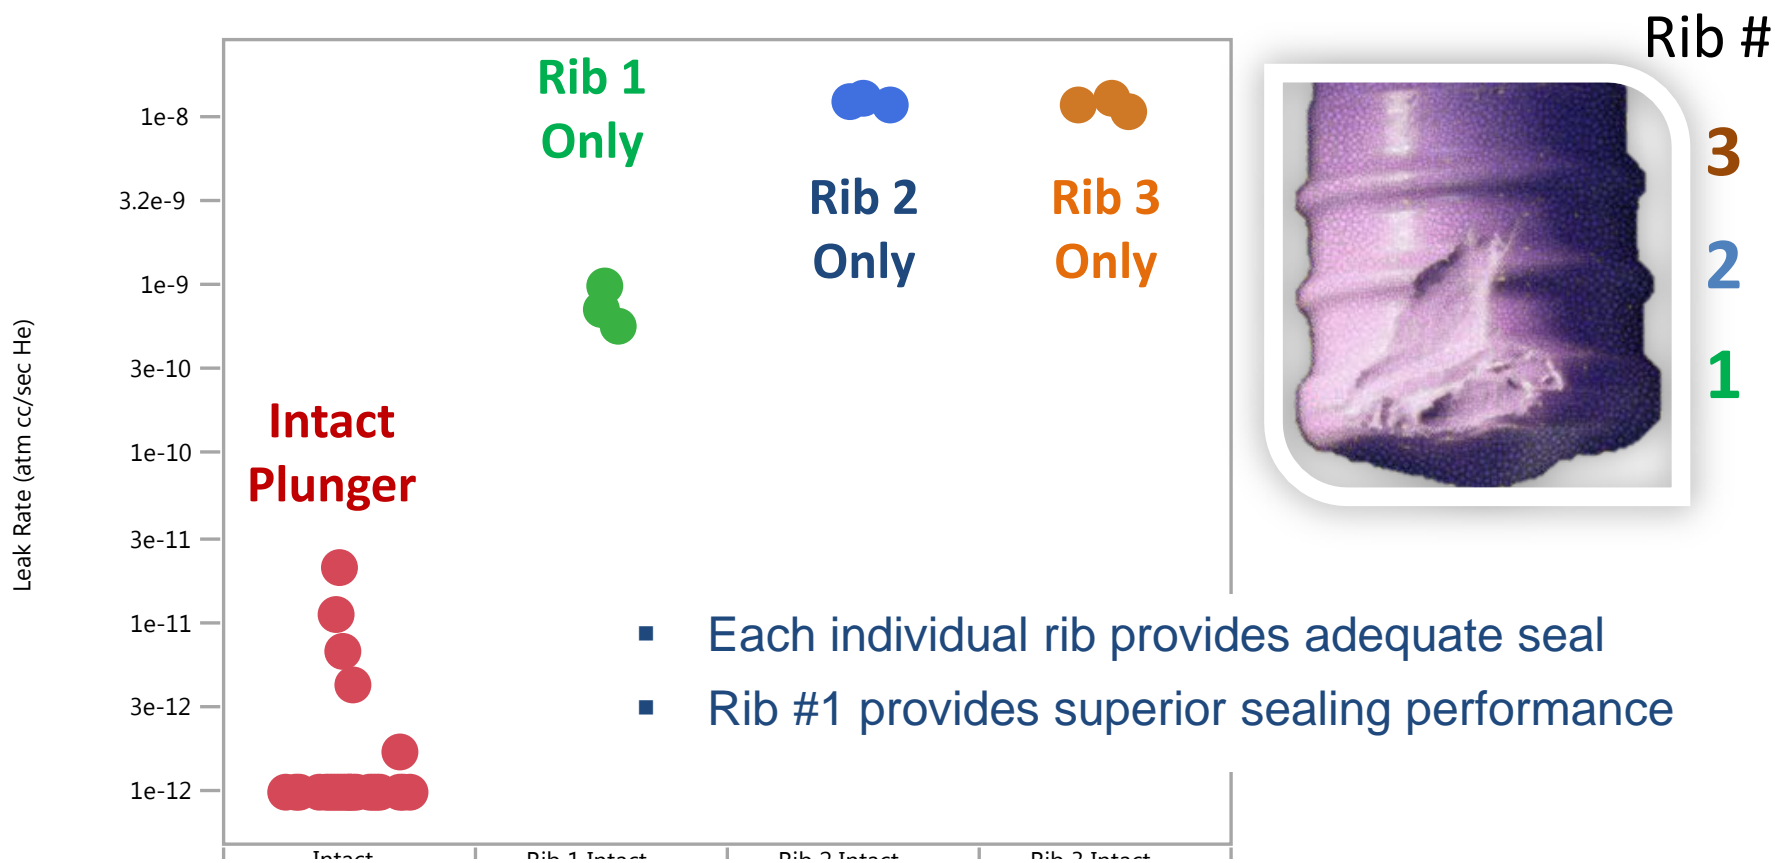





Fiber Interference between plunger rib and barrel

- Industry needs a practical means to fabricate and characterize sub-micron size defects
- Assess impact of interfering fibers of various sizes

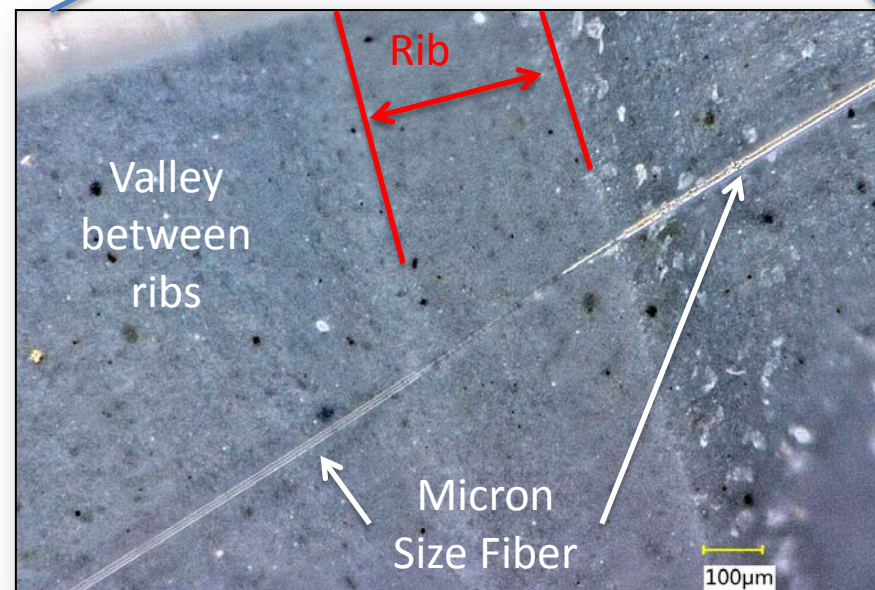


Helium Leakage Rates

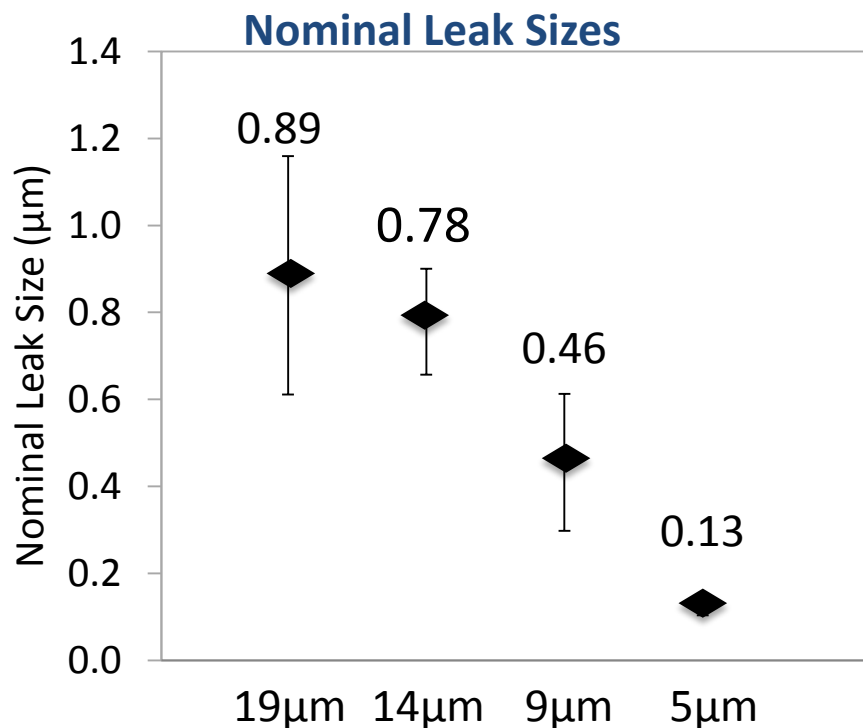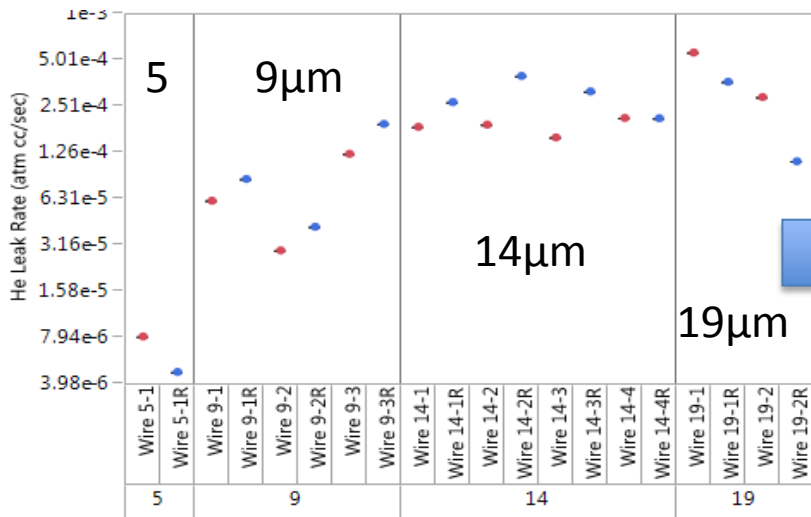

- Presence of interfering fibers could compromise plunger seal integrity
- Interfering fibers provide a practical means for fabricating sub-micron defects
 - Enable development of other CCI testing technologies

Spacer



Needle Shield Gap Study


- How much needle shield movement until it leaks?
- Use spacer to create controlled gaps

“CCI Capability”

- Multiple Lots
- Cpk of leakage rate?
- Correlation with dimensional Cpk

Component aging study

How does the seal performance change over time?

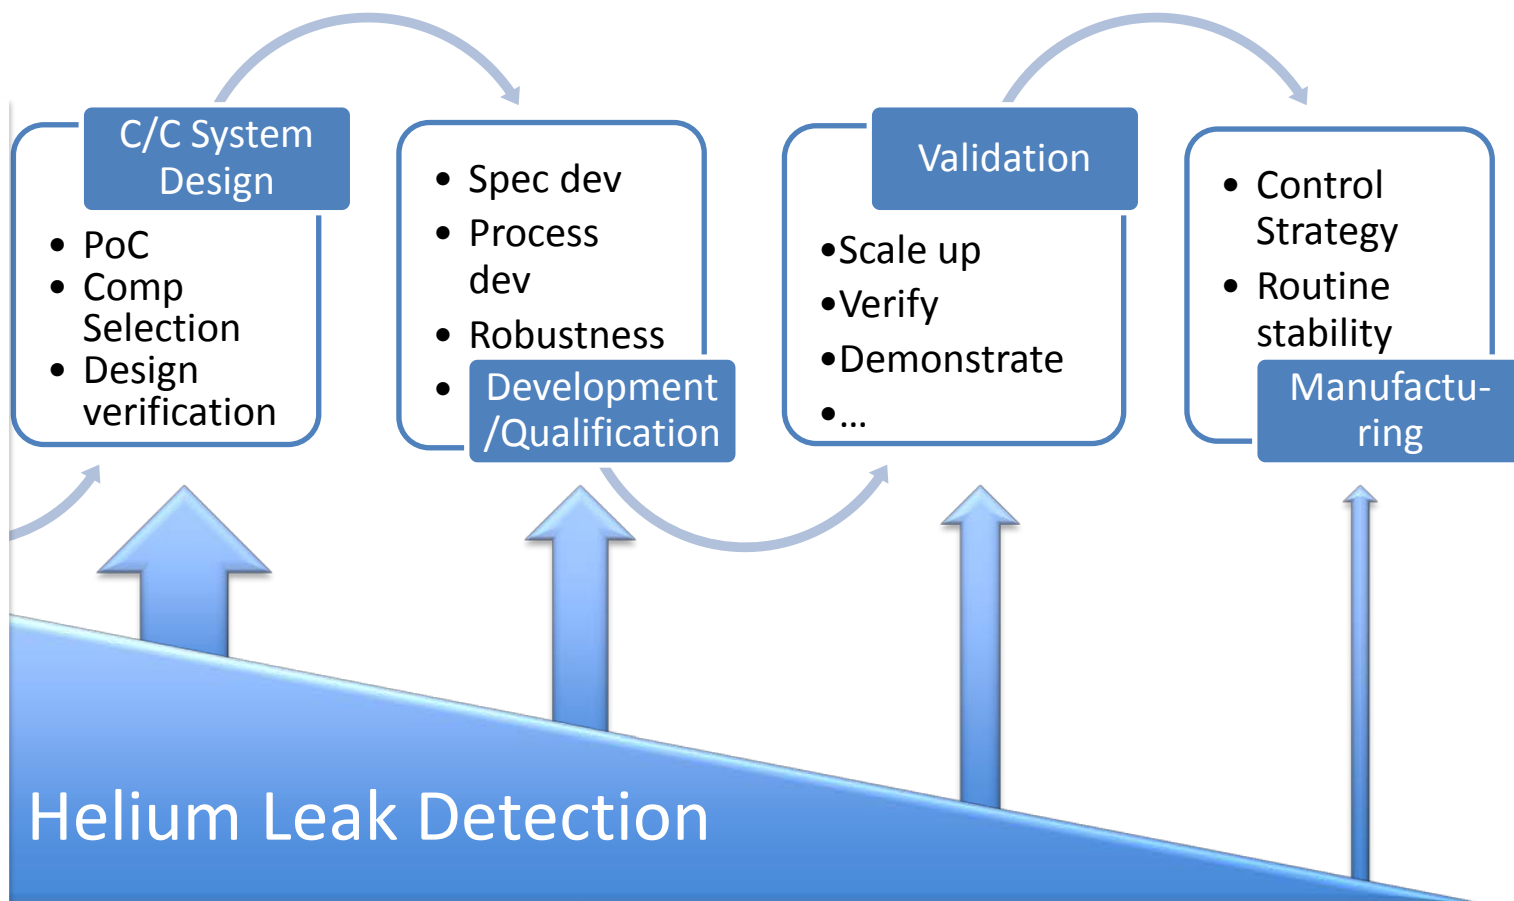

- Sensitive and quantitative testing to inform design & development
- Use in routine manufacturing DP filled container may be limited

Component
Supply

Sealing


Device
Assembly

Packaging

Shipping

Storage

Helium Leak detection

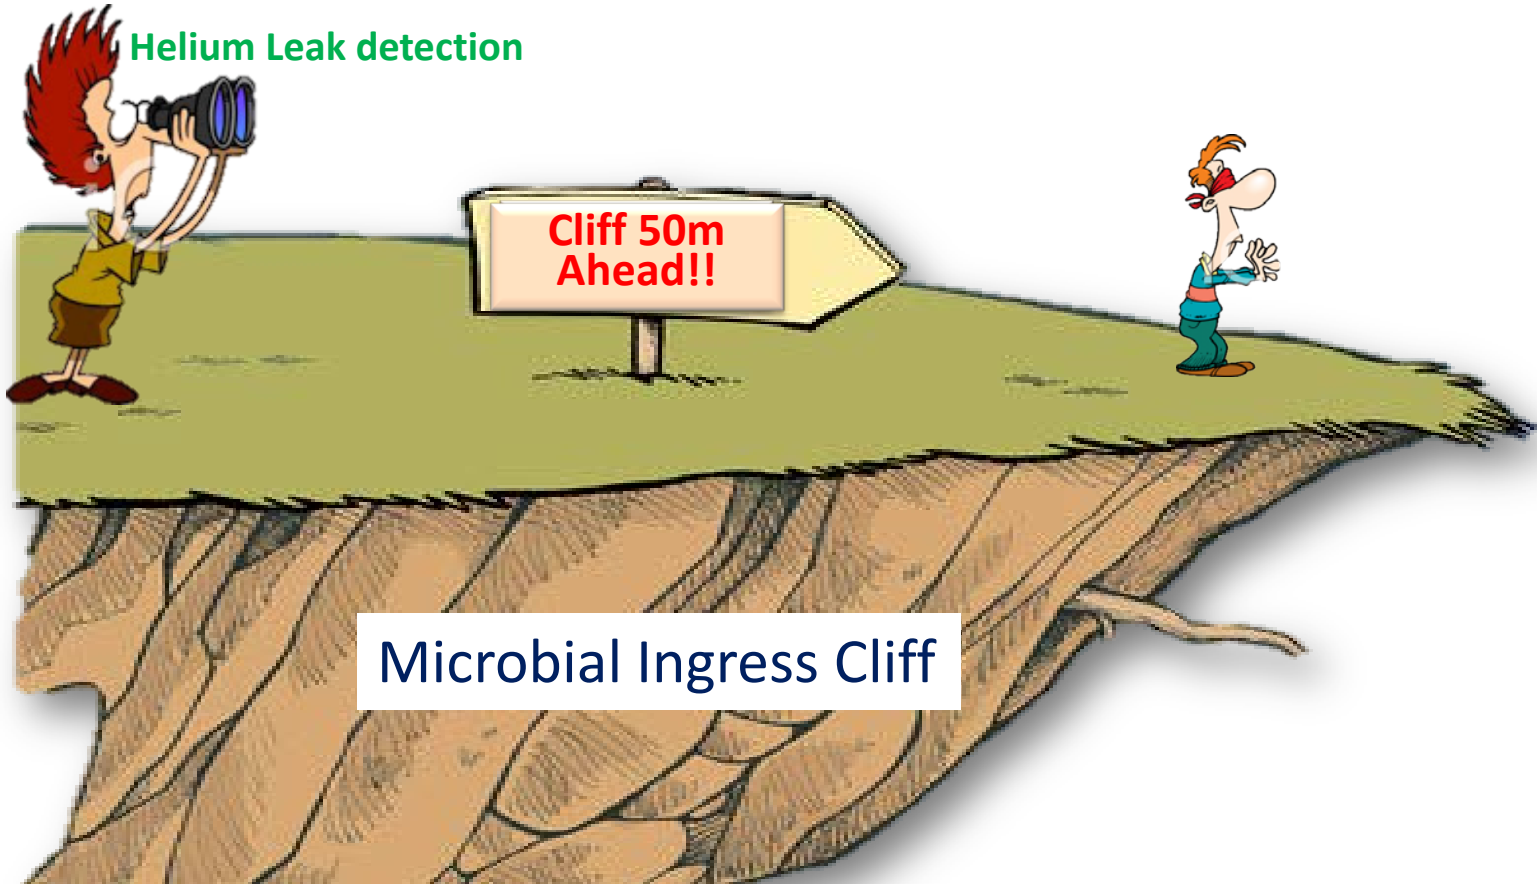

Microbial Ingress Cliff

- ❑ HeLD a capable CCI technology: sensitive, precise, and quantitative
 - Enable data-driven decision making: rich information; high throughput
 - Fixture design and helium charging critical for method development

- ❑ Inform container closure design and process development
 - Inform packaging component selection and system design
 - Assess container closure robustness against design, process variability
 - Demonstrate conformance to MALL

- ❑ Enable foundational CCI research
 - Characterize micron and sub-micron leaks



Acknowledgements

Eli Lilly and Company

Lei Li (co-author)
Li Liu (co-author)
Ross Allen
Lin Li
Jon Parker
Eric Jensen

Ron Iacocca
Andy Ratz
Galen Shi
Karthik Vaideeswaran
Craig Goldhammer

External Collaborators

Elmira Rad, Joseph Buckley, Mike
Berger – Eurofins

Scott Damron & Jason Cumbee
– AGY, Aiken, South Carolina