




Test Methods for Pre-Filled Syringes

Horst Koller, CEO, HK Packaging Consulting GmbH

Roman Mathaes, PhD, Senior Group Leader, Lonza Drug Product Services

PART 5:

- Requirements of the use in devices

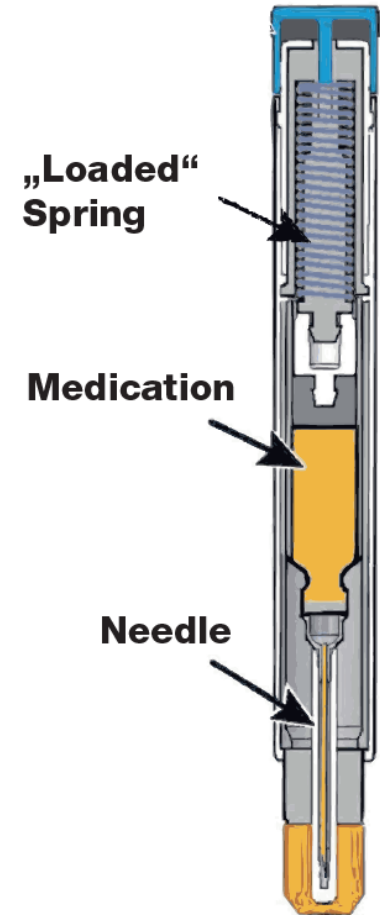

Regulatory References for Finished Pre-filled Syringes in Delivery Devices

ISO 11608-3

**Needle Based Injection Systems (NIS)
for medical use**

Part 3: Finished containers

ISO 11608-3 / Second edition 2012-10-01 (TC 84)

Regulatory References for Delivery Devices

Regulatory Reference: 11608-1 (NIS)

System Designation

- Multi Dose / Single Dose container
- Replaceable / Integrated non replaceable container

- Multi Dose: fixed or variable
- Single Dose: entire / portion of deliverable volume

- Test Matrix and Test Methods:
 - Dose accuracy / last dose accuracy / free fall / conditioning / cyclical / vibration

Pre-filled Container in NIS TM

Regulatory Reference: 11608-3 (NIS)

Requirements

- Freedom from leakage
- Plunger force
- Dimensions
- Eccentricity
- *Meniscus (cartridge only)*
- Resealability

→ pre-requirement is an identified compatible NIS

Pre-filled Container in NIS TM

Regulatory Reference: 11608-3 (NIS)

Requirements

- Coring (fragmentation)
- Particulates
- Dose accuracy / Deliverable volume
- Freedom from damage

→ pre-requirement is an identified compatible NIS

Freedom from leakage TM

Principle

Check if container is tight by applying an axial force via a plunger rod

Procedure

Apply axial pressure: $F = 0.64\text{N/mm}^2 \times (\text{inner diameter})^2$

Hold for 1 min

Interpretation of Results

No leakage visible around front end and back end of container

Plunger force TM

Principle

Check plunger force on open container

Procedure

Use universal tensile and compression machine with recommended test speed of 50mm/min

Record force versus displacement curve

Interpretation of Results

Compare results with pre-defined specification

Dimensions TM

Principle

Check critical dimensions (e.g. plunger insertion depth)

Procedure

Check length of end of FF to back end of plunger

Check length from needle tip to back end of plunger

Check length from tip of septum to back end of plunger

Interpretation of Results

Compare results with pre-defined specification

Resealability TM

Principle

Check tightness of membrane after multiple penetrations

Procedure

Use largest needle provided to system; 29G if not known

Penetrate the septum 1.5 x the maximum number expected

Wipe the septum dry and exert the test force of 5N applied to the plunger

Interpretation of Results

Check for leakage

Coring (Fragmentation) TM

Principle

Check if rubber particles are present after rubber penetration

Procedure

Use NIS system as described in Instruction of Use

Flush lumen of needle after penetration onto a filter

Inspect for rubber particles

Interpretation of Results

Shall not exceed more than 6 fragments / 100 punctures

Particulates TM

Principle

Check for particulate contamination

Procedure

Inspect under normal or corrected-to-normal vision

Interpretation of Results

Shall be essentially free of particulates or droplets (lubrification) on the outside or inside surfaces

Dose accuracy / Deliverable volume TM

Principle

Check dose accuracy assessment matrix in ISO 11608-1

Procedure

Follow informative Annex A / Annex B of ISO 11608-1

Interpretation of Results

Compare results with pre-defined specification

Freedom of damage TM

Principle

Free fall in vertical and horizontal orientation

Procedure

Follow sample preparation and drop orientation as described in section 10.5 of ISO 11608-1

Drop height = 1m

Test surface is a smooth, hard rigid steel (3mm) backed by wood (>10mm)

Interpretation of Results

Compare results with pre-defined specification (breakage)

Workshop: Test Methods for Pre-filled Systems

Additional testing for use in delivery devices

E N D

DISCLAIMER

All interpretations of sample preparation, test procedures and interpretations of results referenced to an ISO standard are the sole interpretation of

HK Packaging Consulting GmbH.

Lonza Drug Product Services

Non limitative list of existing guidelines

Acknowledgements