



HOW TO SET-UP LEACHABLE STUDIES DO'S AND DON'TS

PDA TRAINING COURSE
EXTRACTABLES – LEACHABLES

BASEL
27-28 FEBRUARY, 2020

PIET CHRISTIAENS, PhD



USP<1664> - WHY?

- Assess the potential toxic consequences = **safety**
- Assess impact on the **drug product quality**
- “Real-time” conditions
 - Storage time / temperature / humidity
 - Conditions similar to stability studies
 - Pharmaceutical formulation as contact solution
- The focus is on **quantification** of “**target**” compounds
 - Known polymer additives
 - Validation package of container suppliers
 - **Extractables** study information
- Quantitative aspect: validated methods (ICH Q2 (R1))





Leachables studies can be used to:

- Facilitate timely development of the C/C packaging systems (material selection)
- Establish qual/quant correlations between extractables & leachables
- Establish worst case DP leachables profiles, allowing a safety evaluation on the leachable compounds
- Identify trends in leachable accumulation levels in the drug product over the shelf life
- Facilitate the change control process
- Facilitate investigations into the origin of identified leachables that potentially may cause OOS for a marketed drug product



USP<1664> - WHY?



- For “high risk” dosage forms
 - Pre-clinical stage: selection of packaging components (possible with placebo or simulant)
 - Leachable characterization is recommended for test article batches in **clinical studies** (phase III)
- Post market, supports the change control
 - Changes in formulation
 - Changes in the manufacturing process
 - Changes in primary & secondary packaging or changes in the MoC of components

HOW
TO...



- Will depend upon the drug product

Examples of Packaging Concerns for Common Classes of Drug Products

Degree of Concern Associated with the Route of Administration	Likelihood of Packaging Component-Dosage Form Interaction		
	High	Medium	Low
Highest	Inhalation Aerosols and Sprays	Injections and Injectable Suspensions; Inhalation Solutions	Sterile Powders and Powders for Injection; Inhalation Powders
High	Transdermal Ointments and Patches	Ophthalmic Solutions and Suspensions; Nasal Aerosols and Sprays	—
Low	Topical Solutions and Suspensions; Topical and Lingual Aerosols; Oral Solutions and Suspensions	—	Oral Tablets and Oral (Hard and Soft Gelatin) Capsules; Topical Powders; Oral Powders

- Will **depend upon the purpose and goals** of a leachable study
- However, they require similar types of information
 - Chemical composition of packaging
 - Details of mfg. process
 - Extractables Assessment
 - ALL potential sources should be assessed
 - Primary packaging
 - Secondary packaging (important for semi-permeable containers)
- Nature of contact : direct versus indirect contact (migration mechanism)
- Time of contact: long term vs. transient

HOW
TO...



- Characteristics of the drug product formulation
 - E.g. solid or liquid? (migration mechanism)
- Compounds that may migrate from process materials, may persist through the mfg. process and end up in the final DP: should be treated as leachables!!





Do – Don't #1: Blank solution

What is a good blank solution for leachables testing?

What is a good blank solution for leachables testing?



What is a good blank solution for leachables testing?



- A good blank solution is the real drug product, but without leachables!!

What is a good blank solution for leachables testing?



What do you want to test for?

Yes ✓	No ✗
Leachables from the container closure system	Drug impurities
	Filling line
	Manufacturing equipment
	Degradation products
	Batch variation

What is a good blank solution for leachables testing?



What do you want to test for?

Yes ✓	No ✗
Leachables from the container closure system	Drug impurities
	Filling line
	Manufacturing equipment
	Degradation products
	Batch variation

A good blank solution is a leachables free drug product!!

Most important in the **screening step** in a LEACHABLE Study!


PDA[®] Do – Don't #1: Blank solution

Parenteral Drug Association

What is a good blank solution for leachables testing?



- A good blank solution is a leachables free drug product!!

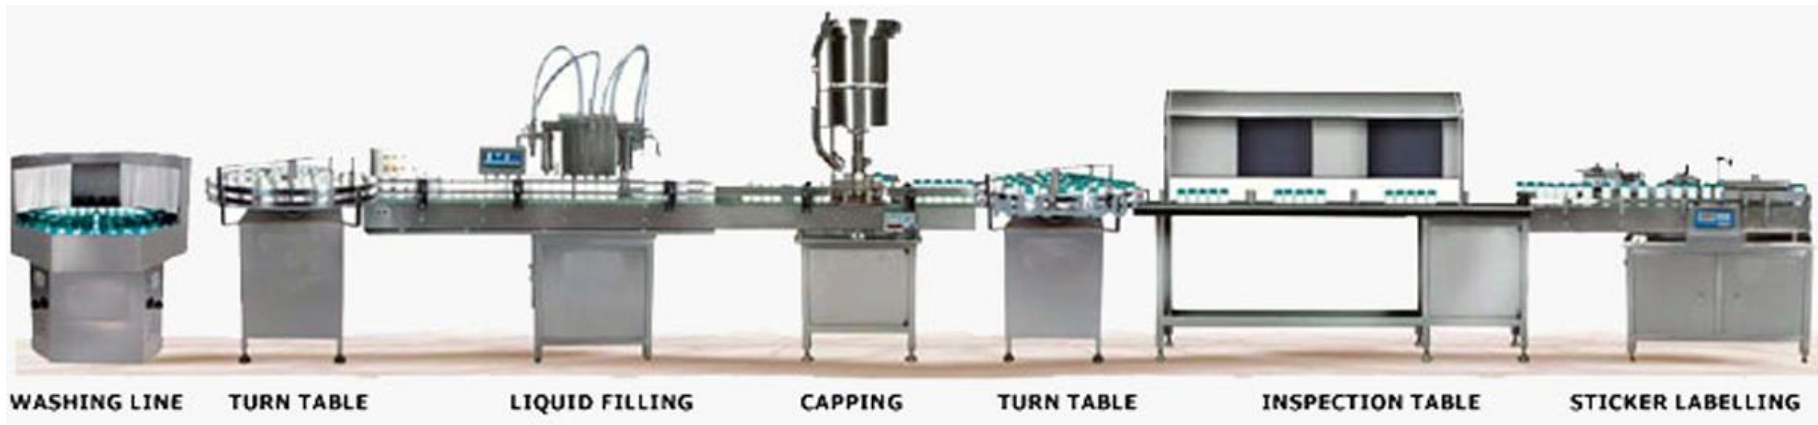


Do – Don't #1: Blank solution

What is a good blank solution for leachables testing?



- A good blank solution is a leachables free drug product!!

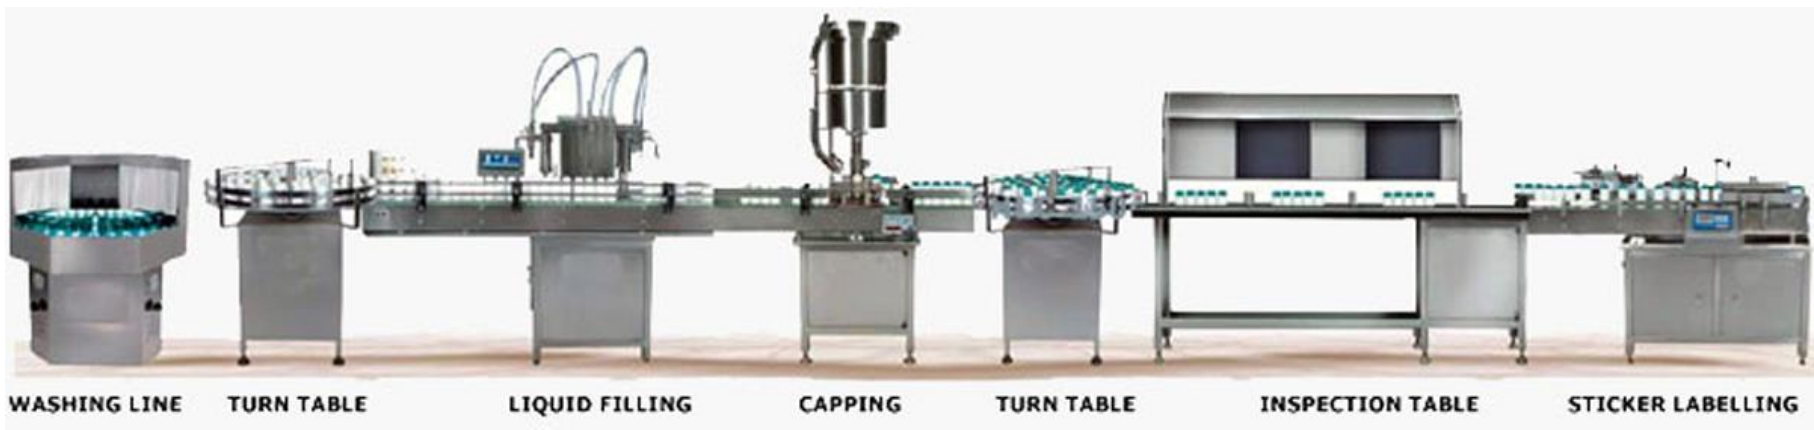

Collect contact samples here




Do – Don't #1: Blank solution

What is a good blank solution for leachables testing?



- A good blank solution is a leachables free drug product!!

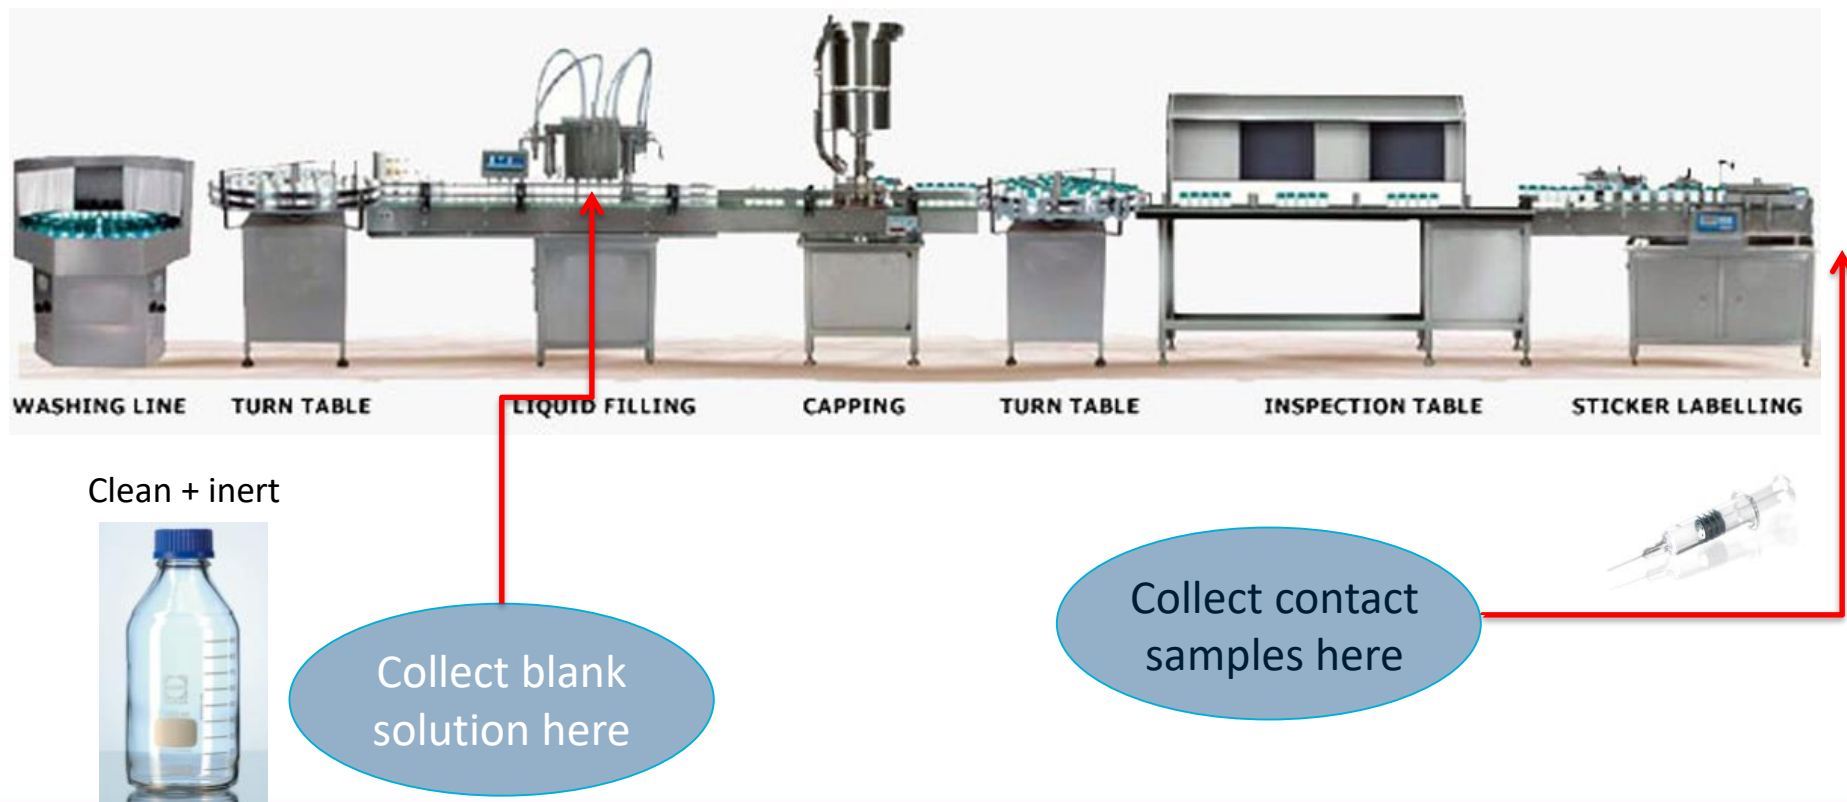


What is a good blank solution for leachables testing?



- A good blank solution is a leachables free drug product!!

Blank
solution

Contact
samples

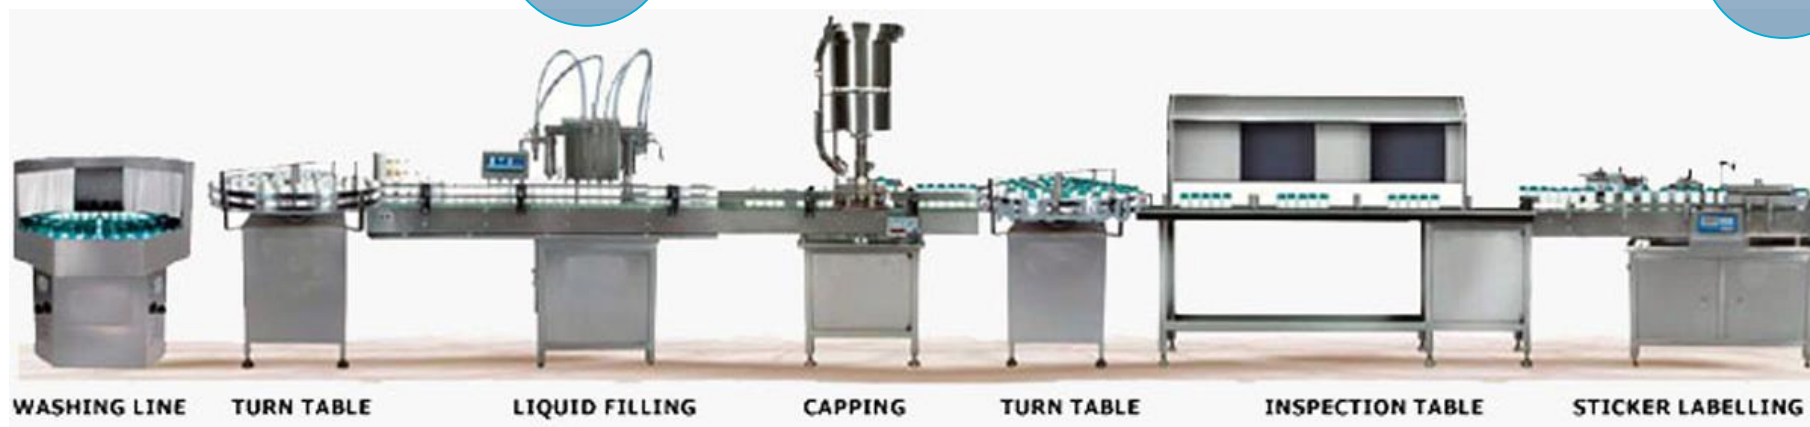


- A good blank solution is best from the same drug product batch as the contact samples

What is a good blank solution for leachables testing?



- A good blank solution is a leachables free drug product!!

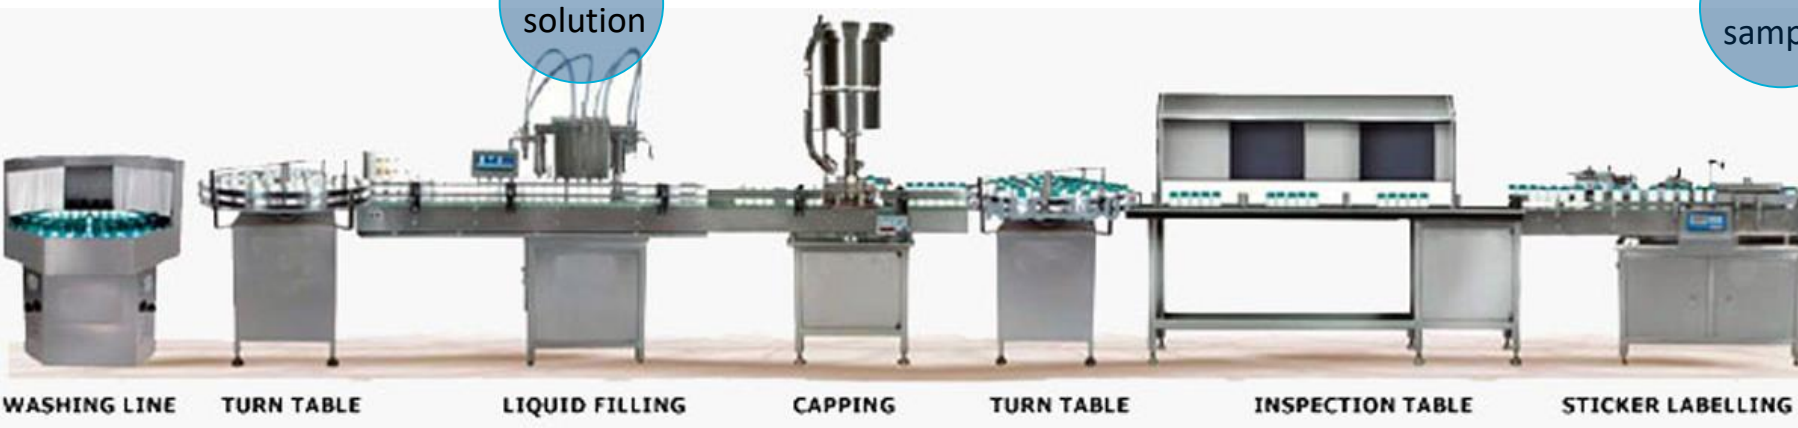


- A good blank solution is best from the **same drug product batch** as the contact samples
- A good blank solution is **put on controlled storage together with the contact samples**

Do – Don't #1: Blank solution


What is a good blank solution for leachables testing?

- A good blank solution is **a leachables free** drug product!!
- A good blank solution is from the **same drug product batch** as the contact samples
- A good blank solution is **put on controlled storage together with the contact samples**

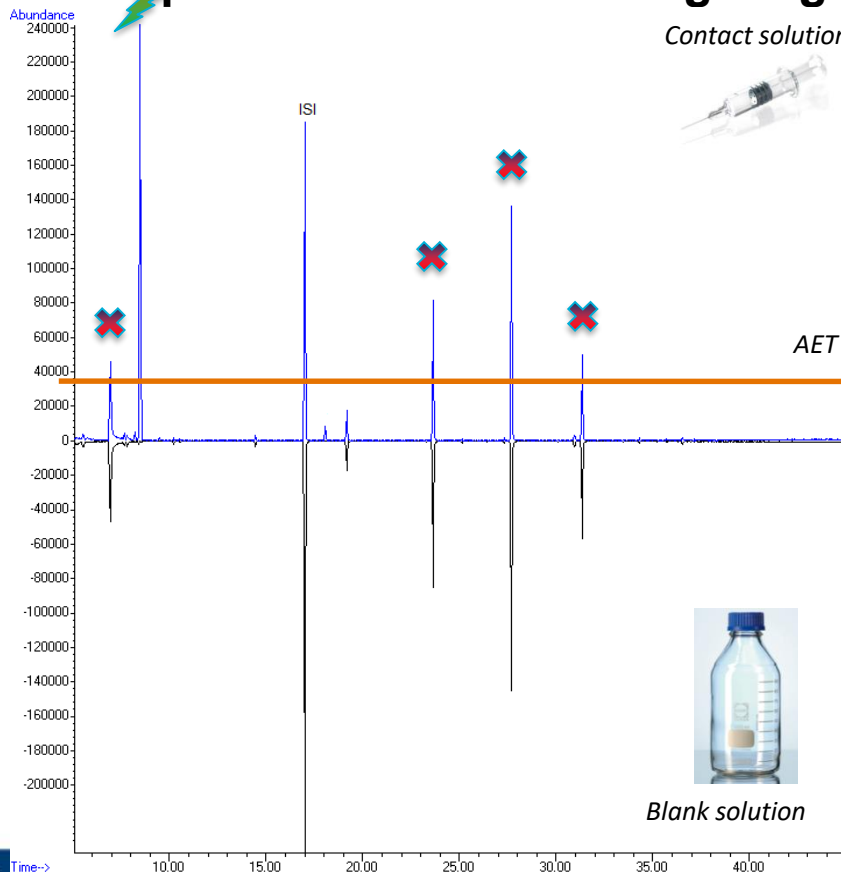

What is a good blank solution for leachables testing?


- A good blank solution is **a leachables free** drug product!!
- A good blank solution is from the **same drug product batch** as the contact samples
- A good blank solution is **put on controlled storage together with the contact samples**

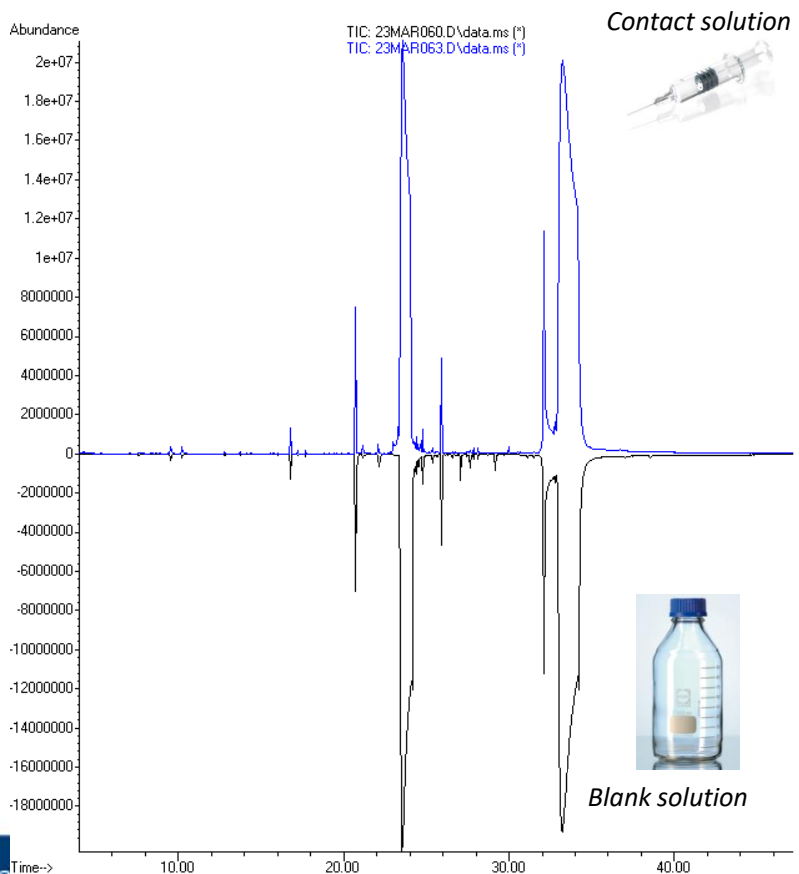

Do – Don't #1: Blank solution

What is a good blank solution for leachables testing?

- A good blank solution is **a leachables free** drug product!!
- A good blank solution is from the **same drug product batch** as the contact samples
- A good blank solution is **put on controlled storage together with the contact samples**

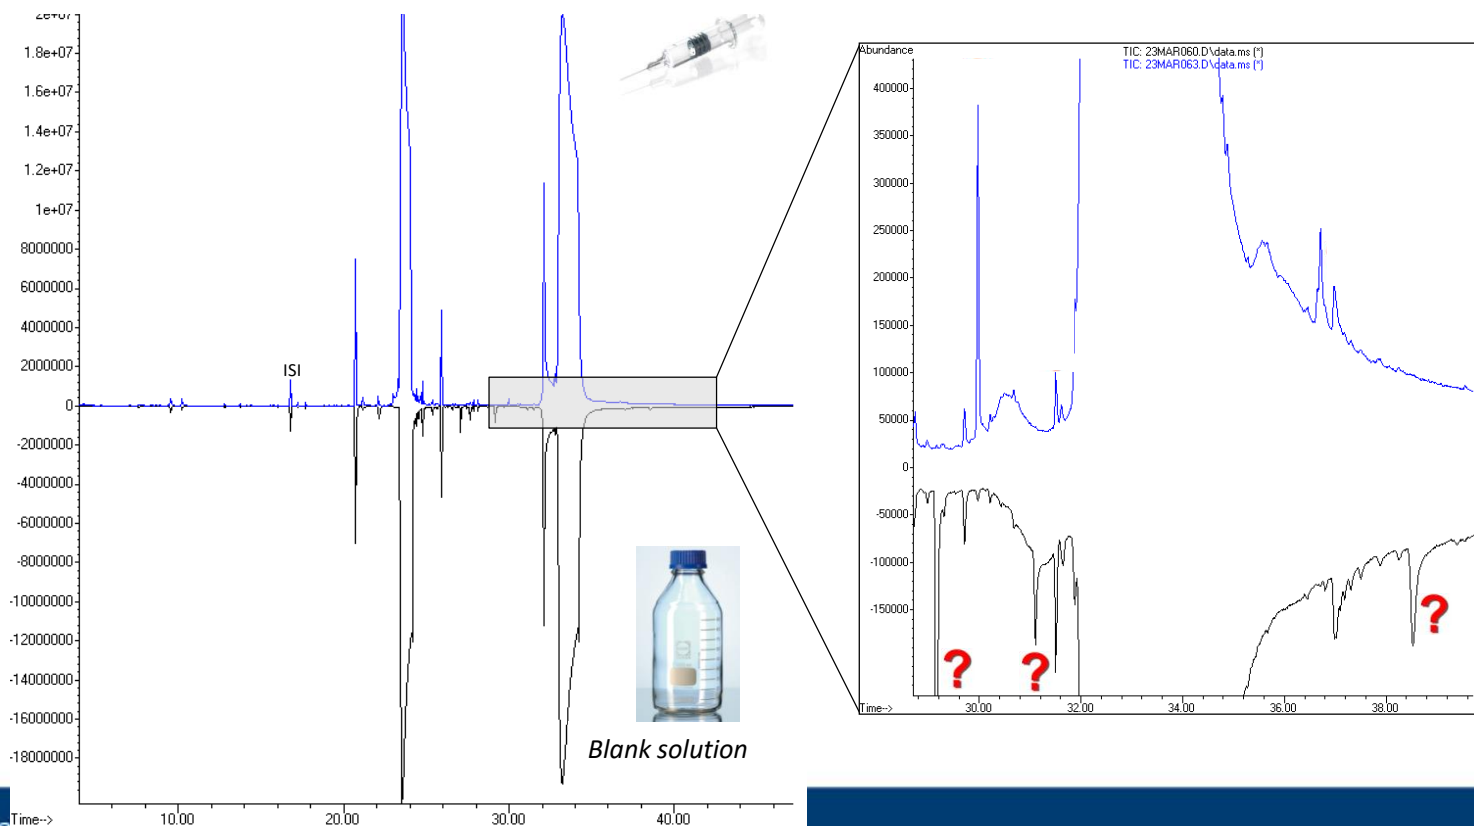

- What the FDA wants....
 - Test multiple batches (3)
- What is a batch?
 - DP batch?
 - Batch of a CCS?
 - Batch of component of a CCS?
 - Batch of the raw material of a component of a CCS?
- Contact your supplier!



Do – Don't #3: Samples

- Sample requirements:
 - Provide sufficient amount of samples
 - Lab work has a large human factor => something can go wrong!
 - Spare samples can save the day!
 - Please don't overkill!!

- Sample requirements:
 - Provide sufficient amount of samples
 - Lab work has a large human factor => something can go wrong
 - Spare samples can save the day!
 - Please don't overkill!!
 - We optimize our capacity for controlled storage











Do – don't #4: Ageing program

- Don't test your drug product only at the end of the shelf life
 - Not only because PQRI and USP<1664> say so...


Do – don't #4: Ageing program

Don't test your drug product only at the end of the shelf life

- Not only because PQRI and USP<1664> say so...

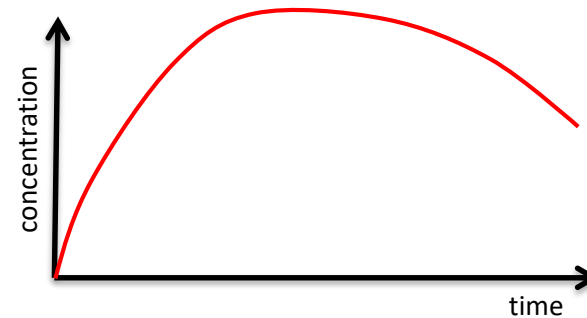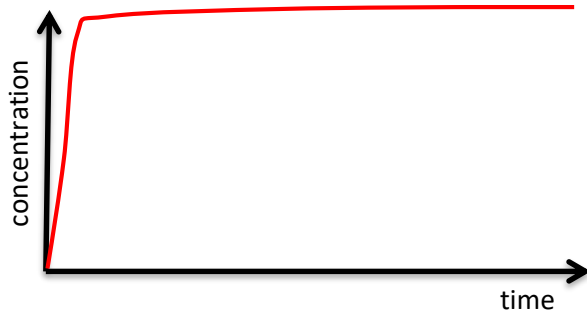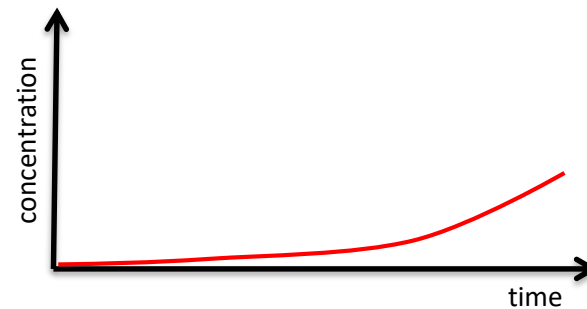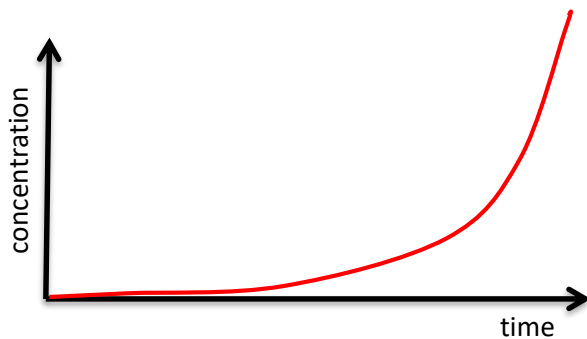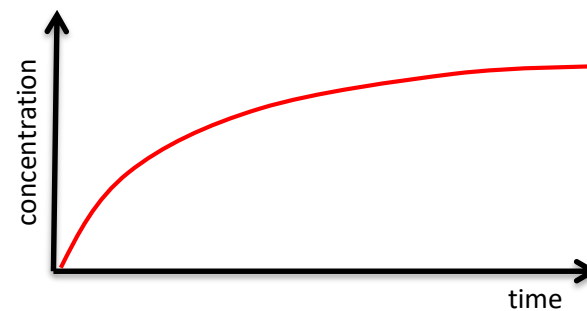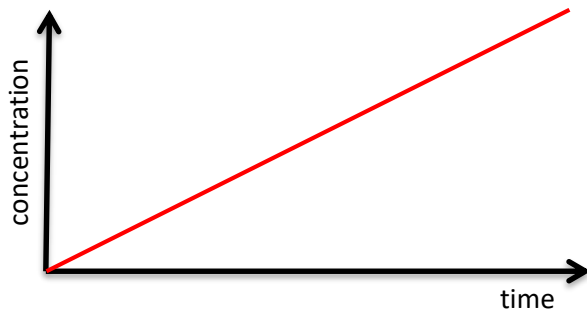


Do – don't #4: Ageing program

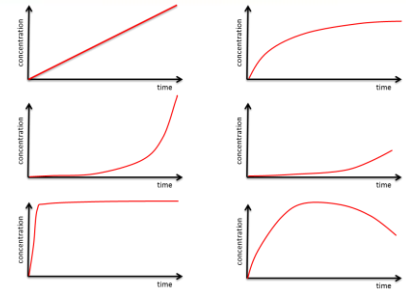

- Don't test your drug product only at the end of the shelf life
 - Not only because PQRI and USP<1664> says so...


- Design an ageing program for specific for your drug product:
 - What is the shelf life?
 - What are the storage conditions?
 - What is the climatic zone of your market?

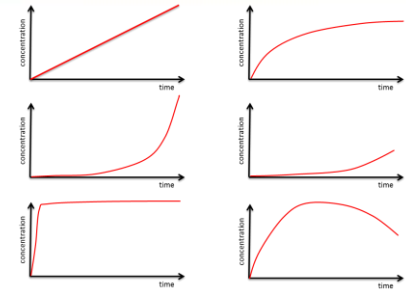

- Don't test your drug product only at the end of the shelf life
 - Not only because PQRI and USP<1664> says so...
- Design an ageing program for specific for your drug product:
 - What is the shelf life?
 - What are the storage conditions?
 - What is the climatic zone of your market?
- Example 1:
 - A product for Belgian market, shelf life = 36 months, storage at ambient temperature

Do – don't #4: Ageing program

- Don't test your drug product only at the end of the shelf life
 - Not only because PQRI and USP<1664> say so...
- Design an ageing program for specific for your drug product:
 - What is the shelf life?
 - What are the storage conditions?
 - What is the climatic zone of your market?
 - Are there specific in-use instructions for the patient?

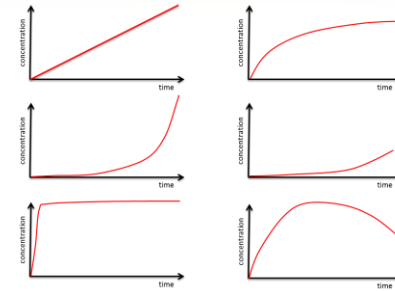


- Example 1:
 - A product for Belgian market, shelflife = 36 months, storage at ambient temperature

	0 months	1 month	3 months	6 months	12 months	18 months	24 months	30 months	36 months	... months
25 °C / 60 % RH	X			X	X	(X)	X		X	
30 °C / 65 % RH										
40 °C / 75 % RH	(X)		X	X						


Do – don't #4: Ageing program

- Don't test your drug product only at the end of the shelf life
 - Not only because PQRI and USP<1664> say so...
- Design an ageing program for specific for your drug product:
 - What is the shelf life?
 - What are the storage conditions?
 - What is the climatic zone of your market?
 - Are there specific in-use instructions for the patient?
- Example 2:
 - A product for Brazilian market, shelflife = 24 months, storage at ambient temperature

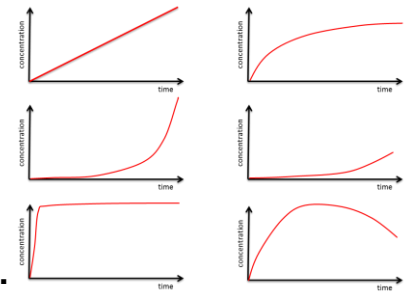

	0 months	1 month	3 months	6 months	12 months	18 months	24 months	30 months	36 months	... months
25 °C / 60 % RH										
30 °C / 65 % RH	X			X	X	X	X			
40 °C / 75 % RH	(X)		X	X						

Do – don't #4: Ageing program

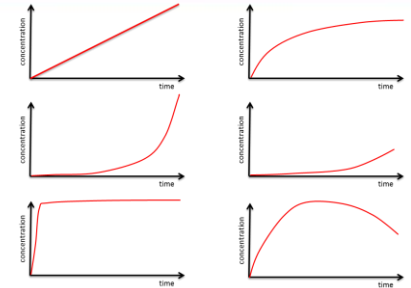


- Don't test your drug product only at the end of the shelf life
 - Not only because PQRI and USP<1664> say so...
- Design an ageing program for specific for your drug product:
 - What is the shelf life?
 - What are the storage conditions?
 - What is the climatic zone of your market?
 - Are there specific in-use instructions for the patient?
- Example 3:
 - A product for Italian market, shelflife = 24 months, storage a 5 °C, in-use for max. 3 months at ambient temperature

	0 months	1 month	3 months	6 months	12 months	18 months	24 months	30 months	36 months	... months
5 °C	X			(X)	X	X	X			
25 °C / 60 % RH	(X)		(X)	X						

Do – don't #4: Ageing program

- Don't test your drug product only at the end of the shelf life
 - Not only because PQRI and USP<1664> say so...
- Design an ageing program for specific for your drug product:
 - What is the shelf life?
 - What are the storage conditions?
 - What is the climatic zone of your market?
 - Are there specific in-use instructions for the patient?

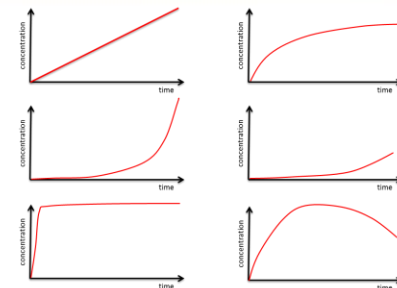

- Example 3:
 - A product for Italian market, shelflife = 24 months, storage a 5 °C, in-use for max. 3 months at ambient temperature

After x months ageing at 5°C, transfer the samples to 25 °C / 60 % RH to simulate the in-use period

	0 months	1 month	3 months	6 months	12 months	18 months	24 months	30 months	36 months	... months
5 °C	X			(X)	X	X	X			
25 °C / 60 % RH	(X)		(X)	X						



Do – don't #5: Quantitative methods?


- How quantitative should the methods to measure the leachables be?
 - Is it always necessary to have fully validated, fully quantitative methods in place?



Do – don't #5: Quantitative methods?


- How quantitative should the methods to measure the leachables be?
- Is it always necessary to have fully validated, fully quantitative methods in place? **No**
- ICH Q2 R1 (Part I, chapter 1):
“The objective of validation of an analytical procedure is to demonstrate that it is suitable for its intended purpose”

- How quantitative should the methods to measure the leachables be?
 - Is it always necessary to have fully validated, fully quantitative methods in place? **No**
 - ICH Q2 R1 (Part I, chapter 1):
“The objective of validation of an analytical procedure is to demonstrate that it is suitable for its intended purpose”
 - Possibilities:
 - Fully validated method according to ICH Q2 R1 (Part II)
 - Complete (linear) method range
 - Known accuracy and precision
 - Limited validation (less parameters of ICH Q2 R1 taken in account)
 - Limit test
 - Method Suitability Test

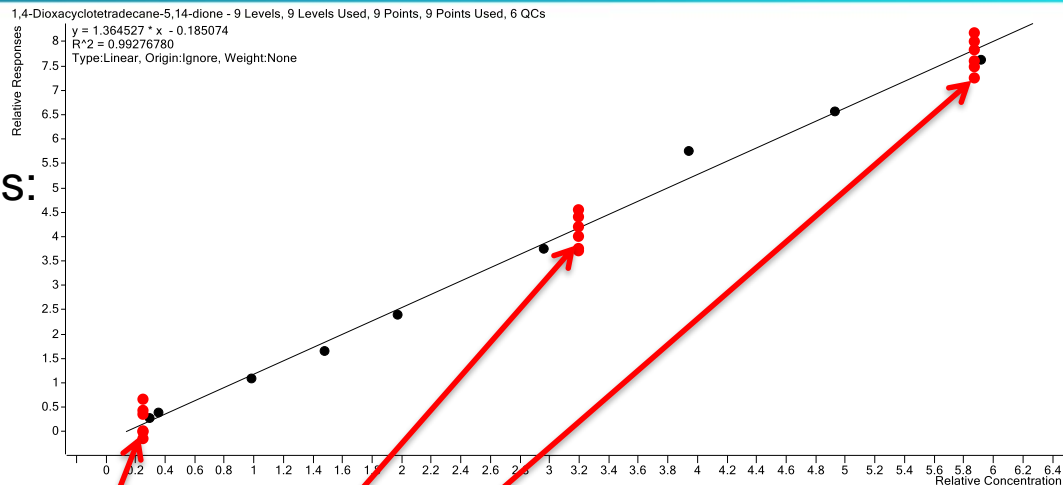


- Fully validated quantitative methods:

low accuracy, low precision




high accuracy, low precision




• = (accepted) true value, n = 6 (average)


low accuracy, high precision




high accuracy, high precision




- Limited validated methods:

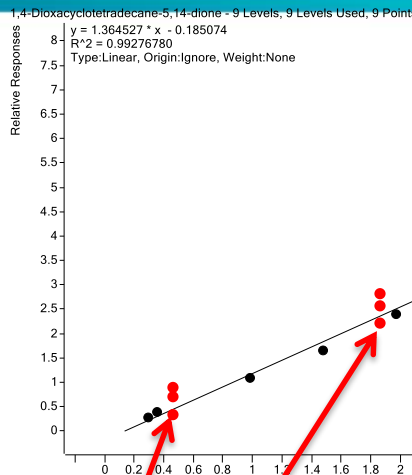

low accuracy, low precision




high accuracy, low precision




• = (accepted) true value, n = 3 (average)


low accuracy, high precision




high accuracy, high precision




- Validated limit test:

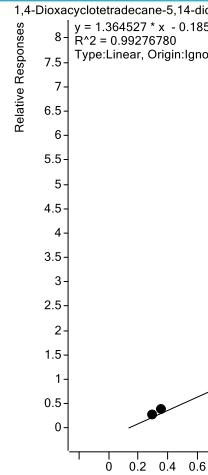

low accuracy, low precision




high accuracy, low precision




• = (accepted) true value, n = 6 (average)


low accuracy, high precision




high accuracy, high precision




- Validated limit test:

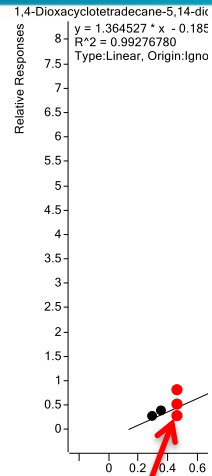

low accuracy, low precision




high accuracy, low precision




• = (accepted) true value, n = 6 (average)

low accuracy, high precision



high accuracy, high precision






Do – don't #5: Quantitative methods?


- Method Suitability Test (MST)? = Cost Friendly and fast alternative to method development and validation
 - Spike analytical standards of the target compounds to a portion blank (leachables free) solution
 - $N = 1$
 - Spike level = AET
 - Spiked samples are treated as other samples
 - MST can prove the detectability of the targets with generic methods

Method Suitability Test (MST)? = Cheap and fast alternative to method development and validation

- Spike analytical standards of the target compounds to a portion blank (leachables free) solution
 - N = 1
 - Spike level = AET
- Spiked samples are treated as other samples
- MST can prove the detectability of the targets with generic methods




Blank solution

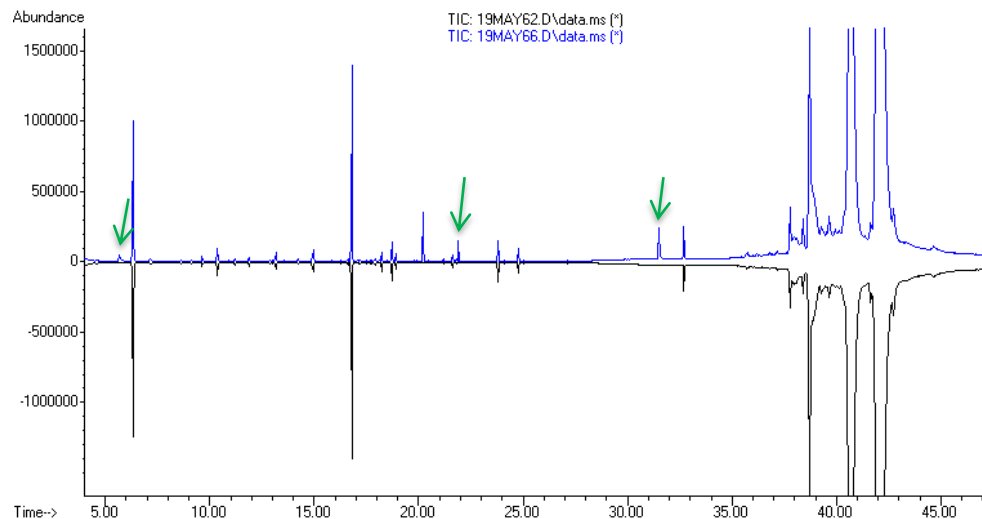


Do – don't #5: Quantitative methods?

- Method Suitability Test (MST)? = Cheap and fast alternative to method development and validation
- Spike analytical standards of the target compounds to a portion blank (leak free) solution
 - N = 1
 - Spike level = AET
- Spiked samples are treated as other samples
- MST can prove the detectability of the targets with generic methods



Blank solution

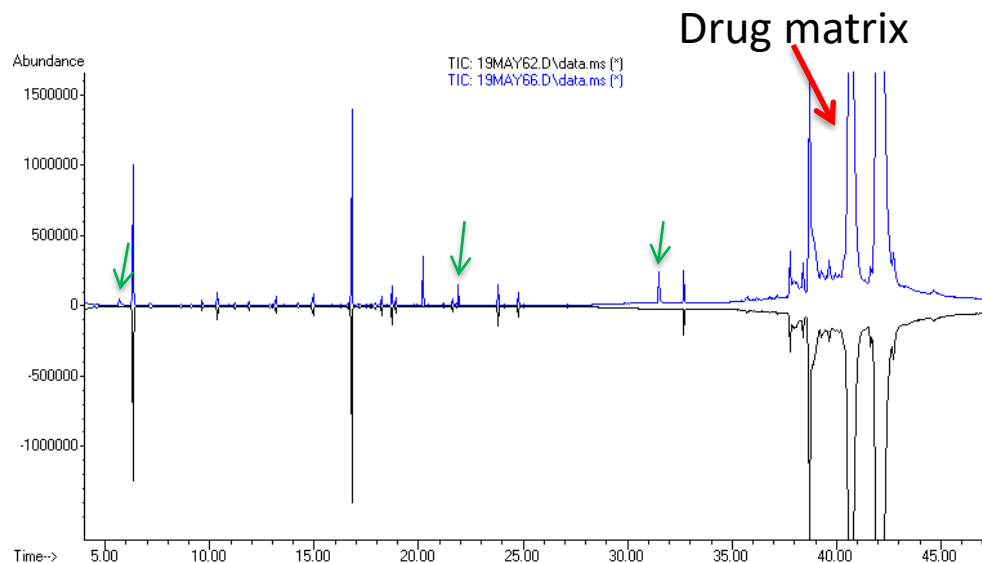

• How quantitative should the methods to measure the leachables be?

- Is it always necessary to have fully validated, fully quantitative methods in place? **No**
 - ICH Q2 R1 (Part I, chapter 1):
“The objective of validation of an analytical procedure is to demonstrate that it is suitable for its intended purpose”
- Possibilities:
 - Fully validated method according to ICH Q2 R1 (Part II)
 - Complete (linear) method range
 - Known accuracy and precision
 - Limited validation (less parameters of ICH Q2 R1 taken in account)
 - Limit test
 - Method Suitability Test
- What should you choose? It depends on
 - Therapy (chronic vs short)
 - Drug product complexity
 - Chance on successful MST on complex drug matrices is rather low
 - Required sensitivity
 - Intended market (USA vs EU vs ...)
 - Company policy
 - ...

The flow of an E&L study: don't forget the screening step!!

Which chemical impurities are migrating into the drug product?

Leachables study

Analysis of the drug product

EXT

TOX

LEA

targeted



Target compounds

Quantitative

Compound-specific thresholds



screening



Unexpected leachables

Semi-Quantitative

Safety Concern Threshold / Qualification Threshold

KEEP IN MIND: FDA (D. Mellon) : All leachables in the DP at $>5\mu\text{g}/\text{day}$ need to be identified
This implicitly calls for a screening step in a leachable evaluation


Screening for **Unexpected Leachables** is considered to be necessary – when (technically) possible

Sources of those “unexpected leachables”:

- Degradation of materials and additives over shelf life, not always accounted in an EXT study
- Degradation, hydrolysis / oxidation of Leachables when present in the DP
- Reactive leachables (reacting with DP ingredients or API)
- ...
- ...
- May address inaccuracies in the study design.

Technically possible means: some DP are too complex in their composition to allow screening at final AET levels.

- Plan ahead!
 - A leachables study design depends on
 - Extractables data
 - Target selection
 - Method development and validation

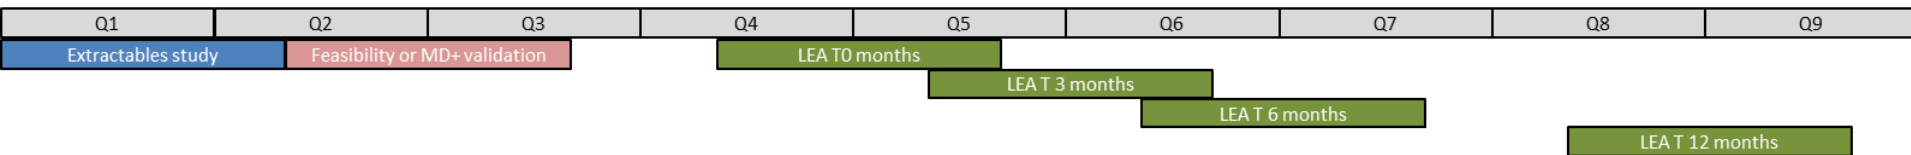

- Differences with a leachables studies
 - The drug product is replaced with a simulating solvent
 - The ageing conditions have been accelerated
 - The test article can be the complete packaging system or a partial packaging system
- Purpose according to USP<1663>
 - Find + identify extractables which are probable leachables
 - Establish which extractables must be targeted in a migration study
 - Screening
 - Mimic circumstances of final drug product: acceleration, moderate exaggeration
 - Worst case: sufficient amounts to identify
 - Safety/ toxicological risk assessment to define target leachables

How to select a simulating solvent?

1. Aqueous based solutions with organic solvent added to mimic the extraction propensity of the actual DP
 - Mix of alcohol in water
 - Nelson Labs Whitepaper (www.nelsonlabs.com)

WHITEPAPER

Establishing the Proper Alcohol/Water Proportion for Simulating Solvents Used in Controlled Extraction Studies

March 25, 2019 | By: Dennis Jenke

The purpose of this paper is to provide guidance on determining the proper alcohol/water proportion for simulating solvents used in controlled extraction studies relevant to drug products that are packaged in plastic container systems, administered via plastic devices or manufactured using systems that consist of plastic components.

2. The drug product vehicle
 - When the DPV is not substantially different from the DP
3. The Drug Product itself
 - “Screening leachable study”

How to select the conditions of a simulation study

1. Exaggerated and accelerated conditions

- Exaggerated:
 - Composition of the simulant
 - Increased surface area
 - Underfilling (bags)
- Accelerated: temperature of storage – accelerated ageing



Only for visualisation – rubber plunger surface area to solution >> 10



2. Study the complete packaging system, not only the individual parts

3. Or study some parts of the packaging system which are of particular interest

Remark: beware of solubility of the extractables in the extraction medium when “back extrapolating” to original ratios

- Regulatory acceptance of a simulation study – **think as a regulator**
 - **Example 1:** use a simulant of 50 % ethanol in water
 - Justifications will need to be provided to prove the predictive character of a simulation study.
 - Secondary leachables – reaction products of leachables with DP – are not covered
 - **CONCLUSION: Risky!**
 - The approach can be taken if a drug formulation is extremely complex and no trace analysis is possible. However, the failed attempts should be documented to help justifying the alternative approach



- Regulatory acceptance of a simulation study – **think as a regulator**
 - Justifications will need to be provided to prove the predictive character of a simulation study compared to a formal leachables study.
 - Only the end point is tested, no trend analysis possible
- **CONCLUSION:** contributes to the E&L assessment, but this is not sufficient!



What if the DP is so complex and challenging in its formulation that a normal analytical approach cannot be taken?

- Try to prove and document the analytical difficulties
- Narrow down the analytics
 - Very targeted, specific compound detection
 - No screening possible
- Consider a simulation study
 - Justify a simulation study by proving the difficulties in the regular leachable study approach

Questions?

